

(19)



Europäische Patentamt
European Patent Office
Office européen des brevets



(11)

EP 0 875 291 A2

(12)

EUROPEAN PATENT APPLICATION

(43) Date of publication

04.11.1998 Bulletin 1998/45

(51) Int Cl⁶ B01L 3/00

// C12Q1/68

(21) Application number: 98303296.2

(22) Date of filing: 28.04.1998

(84) Designated Contracting States:

AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE

Designated Extension States:

AL LT LV MK RO SI

(30) Priority: 02.05.1997 US 850207

02.04.1998 US 53823

(71) Applicant: bioMerieux Vitek, Inc.

Hazelwood, Missouri 63042-2905 (US)

(72) Inventors:

- Catanzariti,Luigi
Duxbury, Massachusetts 02332 (US)
- Klutts,Bryan W.
Norwell, Massachusetts (US)
- McKinley,Geoff A.
Duxbury, Massachusetts (US)
- Garland,Arthur L.
Carver, Massachusetts 02330 (US)

- Graziano,Louis
Rockland, Massachusetts 02370 (US)
- Moe,James G.
Franklin, Massachusetts 02038 (US)
- Vera-Garcia,Marcela
Framingham, Massachusetts 01702 (US)
- Bishop,James Clement
Columbia, Missouri 65203 (US)
- Chastain,David
Acton, Massachusetts 01720 (US)
- Gennari,Fabio
58 50015 Ponte A EMA, Florence (IT)
- Colin,Bruno
69280 Marcy L'Etoile (FR)
- Jaravel,Cecile
69003 Lyon (FR)

(74) Representative: Froud, Clive et al
Elkington and Fife
Prospect House
8 Pembroke Road
Sevenoaks, Kent TN13 1XR (GB)

(54) Dual chamber disposable reaction vessel for amplification reactions, reaction processing station therefor, and methods of use

(57) A reaction vessel for a nucleic acid amplification reaction has a first chamber containing an amplification reagent mix, a second chamber containing an amplification enzyme, and a fluid channel or chamber connecting the first and second chambers together. A fluid sample is introduced into the first chamber. After a denaturation and primer annealing process has occurred in the first chamber, the fluid chamber is opened to allow the solution of the reagent and fluid sample to flow into the second chamber. The second chamber is maintained at an optimal temperature for the amplification reaction.

A station is described for processing test strips incorporating the reaction vessels. The station includes temperature and vacuum control subsystems to maintain proper temperatures in the reaction vessel and effectuate the transfer of the fluid from one chamber to the other in an automated fashion without human intervention.

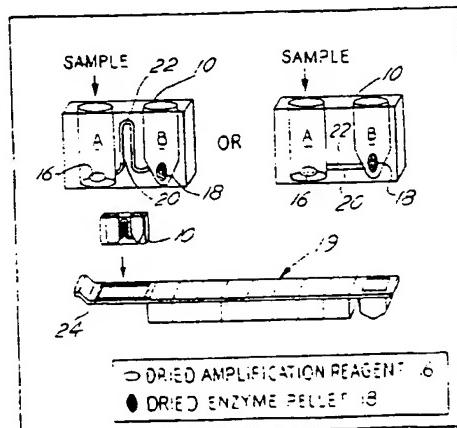


FIG.3

EP 0 875 291 A2

Description

This invention relates to the field of the equipment and methods used for performing nucleic acid amplification reactions. More specifically, the invention relates to a novel disposable dual chamber reaction vessel for a nucleic acid amplification reaction and a station for conducting the reaction in the reaction vessel.

Nucleic acid based amplification reactions are now widely used in research and clinical laboratories for the detection of genetic and infectious diseases. The currently known amplification schemes can be broadly grouped into two classes, based on whether, after an initial denaturing step (typically performed at a temperature of ≥ 65 degrees C) for DNA amplifications or for RNA amplifications involving a high amount of initial secondary structure, the reactions are driven via a continuous cycling of the temperature between the denaturation temperature and a primer annealing and amplification synthesis (or polymerase activity) temperature, or whether the temperature is kept constant throughout the enzymatic amplification process. Typical cycling reactions are the Polymerase and Ligase Chain Reaction (PCR and LCR, respectively). Representative isothermal reaction schemes are NASBA (Nucleic Acid Sequence Based Amplification), Transcription Mediated Amplification (TMA), and Strand Displacement Amplification (SDA). In the isothermal reactions, after the initial denaturation step (if required), the reaction occurs at a constant temperature, typically a lower temperature at which the enzymatic amplification reaction is optimized.

Prior to the discovery of thermostable enzymes, methodologies that used temperature cycling were seriously hampered by the need for dispensing fresh polymerase after each denaturation cycle, since the elevated temperature required for denaturation inactivated the polymerase during each cycle. A considerable simplification of the PCR assay procedure was achieved with the discovery of the thermostable Taq polymerase (from Thermophilus aquaticus). This improvement eliminated the need to open amplification tubes after each amplification cycle to add fresh enzyme. This led to the reduction of both the contamination risk and the enzyme-related costs. The introduction of thermostable enzymes has also allowed the relatively simple automation of the PCR technique. Furthermore, this new enzyme allowed for the implementation of simple disposable devices (such as a single tube) for use with temperature cycling equipment.

TMA requires the combined activities of at least two (2) enzymes for which no optimal thermostable variants have been described. For optimal primer annealing in the TMA reaction, an initial denaturation step (at a temperature of ≥ 65 degrees C) is performed to remove secondary structure of the target. The reaction mix is then cooled down to a temperature of 42 degrees C to allow primer annealing. This temperature is also the optimal reaction temperature for the combined activities of T7

RNA polymerase and Reverse Transcriptase (RT) which includes an endogenous RNase H activity or is alternatively provided by another reagent. The temperature is kept at 42 degrees C throughout the following isothermal amplification reaction. The denaturation step which precedes the amplification cycle, however forces the user to add the enzyme after the cool down period in order to avoid inactivation of the enzymes. Therefore, the denaturation step needs to be performed separately from the amplification step.

In accordance with present practice, after adding the test or control sample or both to the amplification reagent mix (typically containing the nucleotides and the prime), the tube is subject to temperatures ≥ 65 degrees C and then cooled down to the amplification temperature of 42 degrees C. The enzyme is then added manually to start the amplification reaction. This step typically requires the opening of the amplification tube. The opening of the amplification tube to add the enzyme or the subsequent addition of an enzyme to an open tube is not only inconvenient, it also increases the contamination risk.

The present invention avoids the inconvenience and contamination risk described above by providing a novel dual chamber or "binary" reaction vessel, a reaction processing station therefor, and methods of use that achieve the integration of the denaturation step with the amplification step without the need for a manual enzyme transfer and without exposing the amplification chamber to the environment. The contamination risks from sample to sample contamination within the processing station are avoided since the amplification reaction chamber is sealed and not opened to introduce the patient sample to the enzyme. Contamination from environmental sources is avoided since the amplification reaction chamber remains sealed. The risk of contamination in nucleic acid amplification reactions is especially critical since large amounts of the amplification product are produced. The present invention provides a reaction chamber design that substantially eliminates these risks.

In a preferred form of the invention, a dual chamber reaction vessel is provided which comprises a single or unit dose of reagents for a reaction requiring differential heat and containment features, such as a nucleic acid amplification reaction (for example, TMA reaction) packaged ready for use. The dual chamber reaction vessel is designed as a single use disposable unit. The reaction vessel is preferably integrally molded into a test strip having a set of wash and reagent wells for use in a amplification product detection station. Alternatively, the reaction vessel can be made as a stand alone unit with flange or other suitable structures for being able to be installed in a designated space provided in such a test strip.

In the dual chamber reaction vessel two separate reaction chambers are provided in a preferred form of the invention. The two main reagents for the reaction

are stored in a spatially separated fashion. One chamber has the heat stable sample/amplification reagent (containing primers, nucleotides and other necessary salts and buffer components), and the other chamber contains the heat labile enzymatic reagents, e.g. T7 and RT.

The two chambers are linked to each other by a fluid channel extending from the first chamber to the second chamber. A means is provided for controlling or allowing the flow of fluid through the fluid channel from the first chamber to the second chamber. In one embodiment, a membrane is molded into the reaction vessel that seals off the fluid channel. A reciprocable plunger or other suitable structure is provided in the reaction vessel (or in the processing station) in registry with the membrane. Actuation of the plunger causes a breaking of the membrane seal, allowing fluid to flow through the fluid channel. Differential pressure between the two chambers assists in transferring the patient or clinical or control sample through the fluid channel from the first chamber to the second chamber. This can be accomplished by applying pressure to the first chamber or applying vacuum to the second chamber.

Other types of fluid flow control means are contemplated, such as providing a valve in the fluid channel. Several different valve embodiments are described.

In use, the fluid sample is introduced into the first chamber and the first chamber is heated to a denaturation temperature (e.g., 95 degrees C). After the amplification reagents in the first chamber have reacted with the fluid sample and the denaturation process has been completed, the first chamber is quickly cooled to 42 degrees C for primer annealing. The two chambers of the reaction vessel are not in fluid communication with each other prior to completion of the denaturation and cooling step. After these steps are complete, the means for controlling the flow of fluid is operated to allow the reaction solution to pass through the fluid channel from the first chamber to the second chamber. For example, the valve in the fluid channel is opened and the fluid sample is directed into the second chamber either by pressure or vacuum techniques. The reaction solution is then brought into contact with the amplification enzyme(s) (e.g., T7 and/or RT) and the enzymatic amplification process proceeds in the second chamber at 42 degrees C.

In a preferred embodiment, after completion of the reaction, a SPR® (solid phase receptacle) pipette-like device is introduced into the second chamber. Hybridization, washing and optical analysis then proceeds in accordance with well known techniques in order to detect the amplification products.

An integrated stand-alone processing station for processing a reaction in the dual chamber reaction vessel in accordance with presently preferred embodiments of the invention is described. The processing station includes a tray for carrying in proper alignment a plurality of test strips, a temperature control subassembly for maintaining the two chambers of the reaction vessel at

the proper temperatures, a mechanism to open the fluid channel connecting the two chambers together and a vacuum subassembly for providing vacuum to the second chamber to draw the fluid sample from the first chamber into the second chamber.

Presently preferred embodiments of the invention will be described in conjunction with the appended drawings, wherein like reference numerals refer to like elements in the various views, and in which:

Figure 1 is a schematic representation of a disposable dual chamber reaction vessel and the heating steps associated therewith to perform an isothermal amplification reaction, i.e., a TMA reaction, in accordance with one possible embodiment of the invention:

Figure 2 is a schematic representation of alternative form of the invention in which two separate reaction chambers are combined to form a dual chamber reaction vessel:

Figure 3 is a schematic representation of two alternative embodiments of a dual chamber reaction vessel that are snapped into place in a test strip for processing with a solid phase receptacle and optical equipment in accordance with a preferred embodiment of the invention:

Figure 4 is a schematic representation of an alternative embodiment of a dual chamber reaction vessel formed from two separate chambers that are combined in a manner to permit a fluid sample in one chamber to be transferred to the other chamber, with the combined dual chamber vessel placed into a test strip such as illustrated in Figure 3:

Figure 5 is a detailed perspective view of a disposable test strip in which one embodiment of the dual chamber reaction vessel is integrally molded into the test strip at the left-hand end of the test strip:

Figure 6 is detailed perspective view of the disposable test strip of Figure 5 as seen from below:

Figure 7 is a cross section of the disposable test strip of Figures 5 and 6, showing a plunger having a chisel-like tip that is used to pierce a membrane in a fluid channel connecting the two chambers together to thereby allow the fluid to pass from the first chamber into the second chamber:

Figure 8 is a perspective view of the left hand end of the test strip of Figures 5-7 shown enlarged in order to better illustrate the dual chamber reaction vessel:

Figure 9 is a detailed perspective view of a disposable test strip of Figure 5 as seen from below shown greatly enlarged, and with the cap covering the base of the first chamber and intermediate chamber removed:

Figure 10 is a top plan view of the dual chamber reaction vessel of Figures 5-9 shown enlarged:

Figure 11 is a detailed cross section of the dual chamber reaction vessel with the lower cap re-

5 moved as in Figure 9 and with the plunger removed

Figure 12 is a detailed cross section of the dual chamber reaction vessel with the lower cap and plunger installed as they would be in use.

Figure 13 is a perspective view of the plunger of Figure 12:

Figure 14 is another perspective view of the plunger:

Figure 15 is an elevational view of the plunger:

Figure 16 is a perspective view of the cap that covers the base of the first chamber and the intermediate chamber of the reaction vessel of Figures 8 and 9:

Figure 17 is a cross-section of the cap of Figure 16:

Figure 18 is a perspective view of the base of cap of Figure 16:

Figure 19 is a perspective view of a stand-alone disposable dual chamber reaction vessel that is designed to snap into the test strip of the type shown in Figure 5 in the manner suggested in Figure 4:

Figure 20 is a perspective view of the stand-alone disposable dual chamber reaction vessel of Figure 19, with a lower cap as shown in Figures 16-18 removed:

Figure 21 is perspective view of an alternative construction of the stand-alone disposable dual chamber reaction vessel of Figure 19:

Figure 22 is a cross-sectional view of the embodiment of Figure 21:

Figure 23 is a cross-sectional view of the embodiment of Figure 21 showing the action of the helical thimble valve being deformed by a vacuum plunger and the flow of fluid sample from the first chamber into the second chamber:

Figure 24 is a perspective view of the helical thimble valve of Figures 22 and 23:

Figure 25 is a sectional view of the embodiment of Figure 21 showing the flow of fluid through the device from the first chamber into the second chamber:

Figure 26 is a perspective view of another embodiment of the disposable reaction chamber in accordance with the invention designed to snap into the test strip in the manner suggested in Figure 4:

Figure 27 is a cross-section of the embodiment of Figure 26, showing an enzyme plunger carrying an enzyme pellet for introduction into the amplification well

Figure 28 is a cross-section of a test strip incorporating the embodiment of Figure 26. Figures 29A-29C show the use of the test strip of Figure 28.

Figure 30 is a schematic representation of an embodiment of a dual chamber disposable reaction vessel in which a plunger is activated to increase the fluid pressure in the first reaction chamber to break a seal in a fluid channel connecting the first

chamber to the second chamber and force a reaction solution in the first chamber into the second chamber for the amplification reaction to take place. Figure 31 is a perspective view of a stand-alone amplification processing station for the test strips having the dual chamber reaction vessels in accordance with a presently preferred form of the invention:

Figure 32 is a perspective view of one of the amplification modules of Figure 31, as seen from the rear of the module:

Figure 33 is a perspective view of the front of the module of Figure 32:

Figure 34 is another perspective view of the module of Figure 33:

Figure 35 is a detailed perspective view of a portion of the test strip holder and 95 degree C Peltier heating subsystems of the module of Figures 32-34:

Figure 36 is an isolated perspective view of the test strip holder of Figure 35, showing two test strips in accordance with Figure 5 installed in the test strip holder:

Figure 37 is a detailed perspective view of the test strip holder or tray of Figure 33:

Figure 38 is a block diagram of the electronics of the amplification processing station of Figure 33:

Figure 39 is a diagram of the vacuum subsystem for the amplification processing station of Figure 31:

Figure 40 is a graph of the thermal cycle of the station of Figure 31:

Figure 41 is a perspective view of another embodiment of a dual chamber reaction vessel that is suited for use with the test strip of Figure 3 and the reaction processing station of Figures 30-39:

Figure 42 is a vertical sectional view of the vessel of Figure 41 along the line 42-42 of Figure 41:

Figure 43 is a top view of the vessel of Figure 42:

Figure 44 is a detailed illustration of how the conduit and external constriction device work together in a first possible embodiment of the vessel of Figure 41:

Figure 45 is a detailed illustration of how the conduit and external constriction device work together in a second possible embodiment of the vessel of Figure 41:

Figures 46 is a schematic representation of a dual chamber reaction vessel in accordance with one possible embodiment of the invention, with the schematic representation corresponding for example to the embodiment of FIG. 41, and

Figure 47A-47F are schematic drawings showing the different stages of a process for transferring reagent solutions into the vessel and from the first chamber to the second chamber

A preferred form of the invention provides for a dual chamber or "binary" reaction vessel. The term "binary" refers to the characteristic of the vessel of storing in a spatially separated fashion at least two different re-

gents for example a heat stable sample/amplification reagent(s) containing for example primers and nucleotides in one chamber and heat labile enzyme(s) such as T7 and RT in the second chamber. The reagents within the two chambers are not in contact prior to completion of the denaturation and cooling steps. The first chamber is accessible via a pierceable membrane or other means so as to permit a patient or clinical or control sample(s) in liquid form to be added into the first chamber. The second chamber is sealed and contains the enzymatic components of the amplification reaction. The enzymatic components may be in several physical forms, such as liquid, pelletized, lyophilized, etc. After the contents of the first chamber is brought into contact with the second chamber, the reaction can then take place, such as in the second chamber.

In one possible form of the invention, the two chambers may be part of an integrated disposable unit. In another possible embodiment, the two chambers may be two distinct units which have complementary engaging surfaces or features that allow the two units to be combined into a single unit. In the first embodiment, where the two chambers are part of a unitary article, the unit must be made to prohibit the exchange of materials between the two chambers during shipping and prior to the denaturation (heating) step. In both embodiments, a mechanism is required by which the contents of the first chamber (the patient or test sample and amplification reagent(s) mix after denaturation and primer annealing) is brought into contact with the enzyme(s) in the second chamber. The mechanism operates to introduce the contents of the first chamber into the second chamber following the completion of the denaturation step and the cooling of the patient sample/amplification mix to the appropriate temperature for the enzymatic amplification reaction, e.g., 42 degrees C. Several different mechanisms are described in detail herein.

Figure 1 is a schematic representation of a disposable dual chamber reaction vessel 10 and the heating steps associated therewith to perform an isothermal reaction, i.e., a TMA reaction, in accordance with one possible embodiment of the invention. Chamber A contains the amplification reagents or mix, namely deoxynucleotides, primers, MgCl₂ and other salts and buffer components. Chamber B contains the amplification enzyme(s) that catalyzes the amplification reaction, e.g., T7 and/or RT. After addition of the targets (or patient sample) into chamber A, heat is applied to chamber A to denature the DNA nucleic acid targets and/or remove RNA secondary structure. The temperature of chamber A is then quickly cooled down to allow primer annealing. Subsequently the solution of chamber A is brought into contact with chamber B. Chambers A and B, now in fluid communication with each other, are then maintained at the optimum temperature for the amplification reaction, e.g., 42 degrees C. By spatially separating chamber A from chamber B and applying the heat for denaturation to chamber A only the thermolabile enzymes in cham-

ber B are protected from inactivation during the denaturation step.

Figure 2 is a schematic representation of an alternative form of the invention in which two separate reaction chambers 12 and 14 are combined to form a dual chamber reaction vessel 10. Like the embodiment of Figure 1, Chamber A is pre-loaded during a manufacturing step with an amplification reagent(s) or mix, namely nucleotides, primers, MgCl₂ and other salts and buffer components. Chamber B is pre-loaded during manufacturing with the amplification enzyme(s) that catalyzes the amplification reaction, e.g., T7 and/or RT. Fluid sample is then introduced into chamber A. The sample is heated for denaturation of nucleic acids to 95 degrees C in chamber A. After cooling chamber A to 42 degrees C, the solution in chamber A is brought into contact with the enzymes in chamber B to trigger the isothermal amplification reaction.

If the reaction vessel is designed such that, after having brought the contents of chambers A and B into contact, the amplification chamber does not allow any exchange of materials with the environment, a closed system amplification is realized which minimizes the risk of contaminating the amplification reaction with heterologous targets or amplification products from previous reactions or the environment.

Figure 3 is a schematic representation of two alternative dual chamber reaction vessels 10 and 10' that are snapped into place in a test strip 19 for processing with a solid phase receptacle and optical equipment in accordance with a preferred embodiment of the invention. In the embodiments of Figure 3, a unidirectional flow system is provided. The sample is first introduced into chamber A for heating to the denaturation temperature. Chamber A contains the dried amplification reagent mix 16. After cooling, the fluid is transferred to chamber B containing the dried enzyme(s) 18 in the form of a pellet. Chamber B is maintained at 42 degrees C after the fluid sample is introduced into Chamber B. The amplification reaction takes place in Chamber B at the optimum reaction temperature (e.g., 42 degrees C). After the reaction is completed, the test strip 19 is then processed in a machine such as the VIDAS instrument commercially available from biomMérieux Vitek, Inc., Hazelwood, Missouri, the assignee of the present invention. Persons of skill in the art are familiar with the VIDAS instrument.

The unidirectional flow features could be provided by a suitable one-way valve such as check valve 20 in the fluid conduit 22 connecting chambers A and B. The action of transferring the fluid from chamber A to chamber B could be by any of several possible methods such as by introduction of fluid pressure in the solution in chamber A (such as by a piston) or applying a vacuum to chamber B to draw the solution through the fluid channel 22. Examples of these methods are described in detail below.

The steps of heating and cooling of chamber A

could be performed prior to the insertion of the dual chamber disposable reaction vessel 10 or 10' into the test strip 16 or alternatively suitable heating elements could be placed adjacent to the left hand end 24 of the test strip 19 in order to provide the proper temperature control of the reaction chamber A. The stand alone amplification processing station of Figures 31-40, described below, incorporates suitable heating elements and control systems to provide the proper temperature control for the reaction vessel 10.

Figure 4 is a schematic representation of an alternative embodiment of a dual chamber reaction vessel 10" formed from two separate interlocking vessels 10A and 10B that are combined in a manner to permit a fluid sample in one chamber to flow to the other, with the combined dual chamber vessel 10" placed into a test strip 19 such as described above in Figure 3. The fluid sample is introduced into chamber A, which contains the dried amplification reagent mix 16. Vessel A is then heated off-line to 95 degrees C. then cooled to 42 degrees C. The two vessels A and B are brought together by means of a conventional snap fit between complementary locking surfaces on the tube projection 26 on chamber B and the recessed conduit 28 on chamber A. The mixing of the sample solution from chamber A with the enzyme(s) from chamber B occurs since the two chambers are in fluid communication with each other, as indicated by the arrow 30. The sample can then be amplified in the combined dual chamber disposable reaction vessel 10" off-line, or on-line by snapping the combined disposable vessel 10" into a modified VIDAS strip. The VIDAS instrument could perform the detection of the amplification reaction products in known fashion.

Figure 5 is a detailed perspective view of a modified disposable test strip 19 similar to that used in the VIDAS instrument in which a dual chamber reaction vessel 10 comprising a first chamber 32 and a second chamber 34 is integrally molded into the test strip 19 at the left-hand end 24 of the test strip. The test strip 19 includes a plurality of wells to the right of the dual chamber reaction vessel 10. These wells include a probe well 36, a hybridization well 38, an empty well 40, four wash buffer wells 42, 44, 46 and 48, and a well 50 for containing a bleach solution. A substrate cuvette 52 is inserted into the opening 52 at the right hand end 54 of the strip for performance of optical analysis. The test strip 19 is used in conjunction with a SPR®, not shown in the drawings, which is used to draw a fluid sample out of the amplification well 34. The SPR is then dipped into the other wells 36 - 50 during the test procedure in known fashion to perform the analysis for example as performed in the commercially available VIDAS instrument.

Figure 6 is a detailed perspective view of a disposable test strip of Figure 5 as seen from below. Figure 7 is a cross section of the disposable test strip of Figures 5 and 6 showing a plunger 56 having a chisel-like tip at the lower end thereof that is used to pierce a membrane in a fluid channel connecting the two chambers 32 and

34 together to thereby allow the fluid to pass from the first chamber 32 into the second or amplification chamber 34.

Figure 8 is a perspective view of the left hand end of the test strip of Figures 5-7 shown enlarged in order to better illustrate the dual chamber reaction vessel 10. Figure 9 is a detailed perspective view of a disposable test strip of Figure 5 as seen from below shown greatly enlarged, and with a cap 60 (Figure 12) covering the base of the first chamber and the intermediate chamber or fluid channel removed to better illustrate the structure of the device.

Figure 10 is a top plan view of the dual chamber reaction vessel of Figures 5-9 shown enlarged. Figure 11 is a detailed cross-section of the dual chamber reaction vessel with the lower cap removed as in Figure 9, and with the plunger removed. Figure 12 is a detailed cross section of the dual chamber reaction vessel with the lower cap 60 and plunger 56 installed as they would be in use.

Referring to Figures 5-12, the test strip 19 includes a molded body 62 that defines the walls of a reaction vessel 10. The vessel 10 includes a first chamber 32 in which a dried amplification reagent mix is placed at the bottom of the chamber 32 during manufacturing of the test strip 19. Polypropylene is a suitable material for use in molding the device 10 and test strip 19, and a thickness of 40 mils for the walls defining the chambers 32 and 34 is adequate in the illustrated operational embodiment. The wells of the test strip, including the first and second chambers 32 and 34, respectively, are covered with a thin film or membrane 64 after manufacture, shown in Figures 7, 11, 12, to seal all of the wells and reaction vessel 10. The membrane (such as PET, commonly known as MYLAR, or aluminum foil with a more-prime polyethylene/polypropylene mix adhesive) is removed from Figures 5, 8 and 10 in order to illustrate the structures in the test strip 19.

The bottom of the first chamber 32 is capped by a cap 60 that is ultrasonically welded to the bottom surface 68 of the walls defining the first chamber. The cap 60 is shown greatly enlarged in Figures 16-18 and discussed below. The cap 60 provides a fluid passage from the base of the first chamber 32 to the base of an intermediary fluid passage 70 connecting the first chamber 32 to the second chamber 34. A plunger 56 with a chisel-like tip is positioned in the intermediary fluid passage 70. The chisel tip of the plunger 56 breaks a membrane or seal 72 (Figure 9) in the fluid passage (flashed molded in the fluid passage during molding) when the plunger 56 is depressed from above. This allows fluid to migrate from the first chamber 32 into the fluid passage 70 up along the side of the plunger 56 and into a second channel 74 (Figures 8 and 10) communicating with an enzyme pellet chamber 76 that contains the enzyme pellet (not shown). The fluid sample dissolves the enzyme pellet as it travels through the enzyme pellet chamber 76 into the second or amplification chamber 34 (see Figure 8).

A vacuum port 80 (Figure 8) is provided in fluid communication with the second chamber 34. A Porex polyethylene filter (not shown) is positioned within the vacuum port 80. Vacuum is used to effectuate the transfer of the fluid sample from the first chamber 32 to the second chamber 34 after the plunger 56 has been moved to the lower position to break the seal 72. A vacuum implement containing a vacuum probe or tube (see e.g., Figure 33) is inserted into the vacuum port 80 in a manner such that a seal is formed in the top surface 82 of the strip adjacent the vacuum port 80. Vacuum is drawn in the vacuum tube. The pressure difference resulting from ambient pressure in the first chamber 32 and a vacuum in the second chamber 34 draws fluid up the intermediate chamber or fluid passage 70 and into the channel 74 and pellet chamber 76 and into the second chamber 34.

Figure 13 is an isolated perspective view of the plunger 56 of Figure 12. Figure 14 is another perspective view of the plunger 56, shown from below. Figure 15 is an elevational view of the plunger 15. Referring to Figures 13-15, the plunger includes a cylindrically-shaped body 90 having a chisel 92 at the lower end thereof and a head portion 94. The head portion 94 includes a circular ring 96 with voids 98 formed therein to promote the drawing of a vacuum in the intermediate chamber 70 (Figures 8 -12) in which the plunger is installed. The head 94 has downwardly depending feet 100 that seat on a rim 102 (Figure 11) inside the intermediate chamber 70 when the plunger 65 has been depressed to its lowermost position, as shown in Figure 12. The chisel 92 has a tip 104 that breaks through the seal or membrane 72 obstructing the passage of fluid up the intermediate channel 70. The seal 72 is best showing Figures 9, 11 and 12. Figure 12 shows the placement of the chisel 92 just above the seal 72 as it would be while the heating to 95 degrees C in the first chamber 32 is occurring and during the cool-down period.

As shown in Figure 14, the plunger has a V-shaped groove 106 in the side of the plunger body 90 that provides a channel for fluid to rise up the length of the cylindrical body 90 of the plunger to the elevation of channel 74 (Figure 10) connecting the intermediate chamber 70 with the enzyme pellet chamber 76.

Figure 16 is a perspective view of the top surface of the cap 60 that covers the base of the first chamber of the reaction vessel of Figures 8 and 9, shown greatly enlarged. Figure 17 is a cross-section of the cap 60 of Figure 16. Figure 18 is a perspective view of the base of cap 60. Referring to these figures in conjunction with Figures 6 and 9, it will be seen from Figure 8 that without the cap 60 there is no base to the first chamber 32 and no fluid passage between the first chamber 32 and the intermediary chamber 70. The cap 60 provides the base of the first chamber 32 and the passage between the first chamber 32 and the intermediate chamber 70. The cap 60 includes a shallow tray 110 positioned to form a

base of the first chamber 32. The tray 110 slopes downwardly to a small passage 112 linking the shallow tray 110 to a circularly shaped reservoir 114 that is in vertical alignment with the circular wall 116 of the intermediate chamber (see Figure 9). The semirectangular and semicircular rim 118 of the cap 60 is ultrasonically bonded to the bottom portions 68 and 116 of the first and intermediate chambers, respectively, as shown in Figure 6. In the installed condition, when the fluid sample has been introduced into the first chamber 32, the fluid will pass into the channel 112 and reservoir 114, immediately below the seal 72 in the intermediate chamber (see Figure 9). Thus, when the seal 72 is broken by the plunger 56 and vacuum is drawn from the vacuum port 80 of Figure 8, the solution of the fluid sample and reagent from the first chamber 32 will be drawn up the side of the plunger 56 and into the enzyme pellet chamber 76, dissolving the pellet, and into second chamber 34 where the amplification reaction takes place.

Referring to Figure 5, after the amplification reaction has occurred in the second chamber 34 at the proper temperature, the SPR (not shown) is lowered into the second chamber 34 and a portion of the amplified sample is withdrawn into the SPR. The SPR and test strip are moved relative to each other such that the SPR is positioned above the adjacent probe well 36, whereupon it is lowered into the probe well 36. The rest of the analytical processes with the SPR and test strip are conventional and well known in the art. For example, the process may be implemented in the manner performed by the VIDAS instrument of the applicants' assignee.

Figure 19 is a perspective view of a stand-alone disposable dual chamber reaction vessel 10 that is designed to snap into the test strip 19 of the type shown in Figure 5 in the manner suggested in Figure 4. Figure 20 is a perspective view of the stand-alone disposable dual chamber reaction vessel of Figure 19 shown upside down, with a lower cap constructed as shown in Figure 16-18 to cover the base of the first chamber 32 and intermediate chamber 70 removed. A thin film or foil type membrane is applied to the top surface of the reaction vessel 10, in a manner to cover the first chamber 32, the intermediate chamber 34, enzyme pellet chamber 76, second chamber 34 and vacuum port 80. The film is not shown in Figure 19 in order to better illustrate the structures of the reaction vessel 10. Further, a plunger for the intermediate chamber 70 is also not shown. Once the stand-alone disposable reaction vessel of Figures 19 and 20 has been installed into the test strip, the operation of the embodiment of Figures 19 and 20 is exactly as described above.

To accommodate the vessel of Figures 19 and 20 into the test strip 19 of Figures 5 and 6, the test strip 19 is modified by providing an aperture in the left hand end 24 of the test strip adjacent to the probe well 36, and providing suitable rail structures to allow a pair of flanges 120 on the periphery of the unit 10 to snap into the test strip 19. Of course, it will be understood that after mold-

ing of the reaction vessel of Figure 19 the nucleic acid and amplification reagent will be added to the first chamber 32 and the enzyme pellet is added to the enzyme pellet chamber 76. Then the film covering the entire top surface of the vessel 10 will be applied to seal the chambers. The device is then ready for use as described herein.

Figure 21 is perspective view of yet another alternative construction of the disposable dual chamber reaction vessel 10 of Figure 19 that can be molded into a test strip or made as a separate unit to snap into a test strip 19 as described above. The vessel 10 has a first chamber 32 and a second chamber 34 and an intermediate chamber 70 linking the two chambers 32 and 34 together. The base of the first chamber 32 has a hole that is plugged with a cap 60 that is ultrasonically welded to the base of the housing 130. The cap 60 is spaced slightly from the bottom surface of a wall 132 forming the side of the first chamber 32, thereby defining a small passage 134 for fluid to flow out of the first chamber into the intermediate chamber 70. Amplification reagents 16 for the denaturation step are loaded into the base of the chamber 32 of the reaction vessel 10, as shown in Figure 25. An enzyme pellet 18 is loaded into the secondary chamber 34.

An elastomeric thimble-shaped valve element 140 having helical rib features 142, shown isolated in Figure 24, is positioned in the intermediate chamber 70. Figure 22 is a cross-sectional view of the embodiment of Figure 21, showing the thimble valve 140 in the intermediate chamber 70. A filter 144 is positioned above the top of the thimble valve 144. In its relaxed state, a lower circumferential rib 148 on the thimble valve 140 and the exterior surfaces of the helical rib feature 142 on the side walls of the thimble valve 140 make contact with the wall of the intermediate chamber 70, sealing off the chamber 70 and preventing fluid from passing from the gap 134 separating the cap 60 from the wall 132, up the intermediate chamber 70 and into the secondary chamber 34.

The resilient thimble valve 140 is deformable such that the lower circumferential rib 148 may be moved away from the wall of the intermediate chamber 70. This is achieved by inserting an element 152 into the interior of the thimble valve 140 and pressing on the wall portion 149 of the valve 140 to stretch and deform the end wall and adjacent shoulder of the thimble valve. Figure 23 is a cross-sectional view of the embodiment of Figure 21 showing the action of the helical thimble valve 140 being deformed by a vacuum plunger 152 that is inserted into the interior of the thimble valve 140. The end of the vacuum plunger presses against the wall 149 as shown in Figure 23, pulling the lower circumferential rib away from the wall of the intermediate chamber 70. The helical rib feature 142 stays in contact with the cylindrical wall of the chamber 70. At the same time, vacuum is drawn through an aperture in the side of the vacuum plunger 152 to pull air out of the secondary chamber 34 and through the filter 144 into the vacuum plunger 152.

This vacuum action draws fluid out of the base of the first chamber 32 and up vertically in a helical path along the helical port defined between the helical rib feature 142 and the wall of the intermediate chamber 70. Substantially all of the patient sample/reagent solution in the first well 32 is removed in accordance with this embodiment. The solution passes from the upper end of the helical feature 142 into a gap 150 connecting the intermediate chamber 70 with the second chamber 34. This is illustrated best in Figures 23 and 25.

The embodiment of Figures 21-23 has the advantage that the opening of the thimble valve 140 tends to cause any oil in the amplification reagent mix in the first chamber that may find its way to the base of the intermediate chamber 70 to be blown back toward the first chamber, acting in the manner of a common plunger, and allow the fluid sample and reagent solution to take its place. Where the amplification reagent contains an oil such as a silicone oil, it is important that the oil is not the first substance to migrate into the second chamber, as this can cause the oil to coat the enzyme pellet in the second chamber, which can interfere with the amplification reaction in the second chamber 34. Thus, preferably the thimble valve 140 is designed such that when the wall 149 of the thimble valve 140 is activated by the vacuum probe 152, any oil that may lie at the base of the intermediate chamber 70 is initially forced back into the first chamber 32. Once the lower rib 148 of the thimble valve 140 is moved away from the wall of the intermediate chamber 70, the drawing of the vacuum in the second chamber allows the fluid sample/reagent solution to be drawn into the second chamber as described above.

Figure 26 is a perspective view of yet another embodiment of the disposable reaction vessel 150 in accordance with the invention. The reaction vessel 150 is designed to snap into the test strip 19 of Figure 8 in the manner suggested in Figure 4 and described above. Figure 27 is a cross-section of the embodiment of Figure 26. Referring to Figures 26 and 27, the disposable reaction vessel 150 comprises a unitary housing 152 that defines a first chamber or amplification well 154 which has loaded in it an amplification pellet or dried reagent mix 16 for the denaturation step in the TMA process. The amplification well 154 is separated from a second chamber 156 by a heat and moisture isolation barrier 158. The second chamber contains an enzyme plunger or carrier 160 for containing an enzyme pellet 18 for introduction into the amplification well 154 after the fluid sample has been introduced into the amplification well 154 and the denaturation process has been completed. The enzyme plunger 160 has a recessed surface 162 for receiving an implement through the opening at the top of the chamber 156. A foil layer 164 is applied to the top surface of the reaction vessel 150 as shown.

Figure 28 is a cross-section of a test strip 19 incorporating the embodiment of Figure 26. The reaction vessel 150 can be manufactured as a stand-alone disposable unit as suggested in Figures 26 or 27 and snapped

into place in a test strip as shown in Figure 28 or the test strip of Figure 28 may be manufactured with the amplification well of Figure 31 as an integral part of the test strip 19 itself. In the preferred embodiment, the unit 150 is manufactured as an integral part of the test strip. The test strip 19 has a sliding cover 164 positioned at the end of the test strip 19 comprising a gripping surface 166 and a plastic label 168 carried by first and second mounting structures 170.

Figures 29A-29C show the use of the test strip 19 with the disposable reaction vessel of Figure 28. In the first step, the sliding cover 164 is pulled back and a pipette 172 is inserted through the foil layer 164 to deposit the fluid sample 176 into the amplification well 154. The pipette 172 is removed and the cover 164 is slid back into place over the amplification well 154 into the position shown in Figure 29B. The amplification well 154 is heated to 95 degrees C to subject the fluid sample 176 to denaturation with the aid of the amplification reagent pellet 16. The second chamber 156 containing the enzyme pellet 18 is not subject to the 95 degree C heating. After the amplification well has cooled down to 42 degrees C, an implement 180 is inserted into the second chamber containing the enzyme carrier 160 and enzyme pellet 18 and placed into contact with the enzyme carrier 160. The implement 180 is moved further in to force the carrier 160 through the heat and moisture isolation barrier 158, thereby adding the enzyme pellet 18 to the amplification well 154. The enzyme carrier 160 blocks the chamber as shown in Figure 29 C, preventing contamination of the amplification well 154. A cover (not shown) could be slid over the entrance of the second chamber or channel if desired. The amplification well 154 is then maintained at a temperature of 42 degrees C for roughly one hour for the amplification process to proceed. After the amplification process is complete, a reagent SPR having at least one reaction zone is inserted through a membrane 168 or label as shown in Figure 29 C, and a portion of the amplified solution is withdrawn into the SPR. The rest of the process proceeds in known fashion.

Figure 30 is a schematic representation of yet another embodiment of a dual chamber disposable reaction vessel 10. The fluid sample is loaded into the first chamber 32 and denaturation and primer annealing steps are performed in the first chamber 32, with the aid of an amplification mix reagent loaded into the first chamber. After the first chamber has cooled to 42 degrees C, a piston mechanism 184 is applied to the first chamber 184 to increase the fluid pressure in the first reaction chamber to break a seal 186 in a fluid channel 188 connecting the first chamber 32 to the second chamber 34. The fluid sample is forced from the first chamber 32 into the second chamber 34. The second chamber is loaded with the enzyme pellet 18. The amplification reaction takes place in the second chamber 34 at a temperature of 42 degrees C. The piston 184 may be incorporated as a cap structure to the reaction

vessel 10 and which is depressed by a SPR as shown or a separate piston could be used to force the fluid from the first chamber 32 into the second chamber 34.

Figure 31 is a perspective view of a stand-alone amplification reaction processing system 200 for the test strips 19 (see, e.g., Figures 3 and 5) having the dual chamber reaction vessels in accordance with a presently preferred form of the invention. The system 200 consists of two identical amplification stations 202 and 204, a power supply module 206, a control circuitry module 208, a vacuum tank 210 and connectors 212 for the power supply module 206. The tank 210 has hoses 320 and 324 for providing vacuum to amplification stations 202 and 204 and ultimately to a plurality of vacuum probes (one per strip) in the manner described above for facilitating transfer of fluid from the first chamber to the second chamber. The vacuum subsystem is described below in conjunction with Figure 39.

The amplification stations 202 and 204 each have a tray for receiving at least one of the strips 19 of Figure 5 (in the illustrated embodiment up to 6 strips) and associated temperature control, vacuum and valve activation subsystems for heating the reaction wells of the strip to the proper temperatures, effectuating a transferring of fluid from the first chamber in the dual chamber reaction wells to the second chamber, and activating a valve such as a thimble valve in the embodiment of Figure 22 to open the fluid channel to allow the fluid to flow between the two chambers.

The stations 202 and 204 are designed as stand alone amplification stations for performing the amplification reaction in an automated manner after the patient or clinical sample has been added to the first chamber of the dual chamber reaction vessel described above. The processing of the strips after the reaction is completed with a SPR takes place in a separate machine, such as the commercially available VIDAS instrument. Specifically, after the strips have been placed in the stations 202 and 204 and the reaction run in the stations, the strips are removed from the stations 202 and 204 and placed into a VIDAS instrument for subsequent processing and analysis in known fashion.

The entire system 200 is under microprocessor control by an amplification system interface board (not shown in Figure 31). The control system is shown in block diagram form in Figure 38 and will be described later.

Referring now to Figure 32, one of the amplification stations 202 is shown in a perspective view. The other amplification station is of identical design and construction. Figure 33 is a perspective view of the front of the station 202 of Figure 31.

Referring to these figures, the station includes a vacuum probe slide motor 222 and vacuum probes slide cam wheel 246 that operate to slide a set of vacuum probes 244 (shown in Figure 33) for the thimble valves of Figure 21 up and down relative to a vacuum probes slide 246 to open the thimble valves (reference 140 in

- the embodiment of Figures 21-23) and apply vacuum so as to draw the fluid from the first chamber of the reaction vessel 10 (e.g. Figure 21) to the second chamber. The vacuum probes 244 reciprocate within annular recesses provided in the vacuum probes slide 246. The vacuum probes 244 are positioned in registry with the intermediate chamber 70 in the embodiment of Figure 22 or in registry with the vacuum port 80 in the embodiment of Figure 11.

For an embodiment in which the strips are constructed in the manner of Figures 5-12, the vacuum probe 244 would incorporate a suitable pin structure (not shown) immediately adjacent the shaft of the vacuum probe 244 that would operate the plunger 56 of Figure 12 to open the intermediate chamber 70 when the vacuum probe 244 is lowered onto the vacuum port. Obviously, proper registry of the pin structure and vacuum probe 244 with corresponding structure in the test strip as installed on the tray needs to be observed.

The station includes side walls 228 and 230 that provide a frame for the station 202. Tray controller board 229 is mounted between the side walls 228 and 230. The electronics module for the station 202 is installed on the tray controller board 229.

A set of tray thermal insulation covers 220 are part of a thermal subsystem and are provided to envelop a tray 240 (Figure 33) that receives one or more of the test strips. The insulation covers 220 help maintain the temperature of the tray 240 at the proper temperatures. The thermal subsystem also includes a 42 degree C Peltier heat sink 242, a portion of which is positioned adjacent to the second chamber in the dual chamber reaction vessel in the test strip to maintain that chamber at the proper temperature for the enzymatic amplification reaction. A 95 degree C heat sink 250 is provided for the front of the tray 240 for maintaining the first chamber of the reaction well in the test strip at the denaturation temperature.

Figure 34 is another perspective view of the module of Figure 33, showing the 95 degree C heat sink 250 and a set of fins 252 dissipating heat. Note that the 95 degree C heat sink 250 is positioned to the front of and slightly below the tray 240. The 42 degree C heat sink 242 is positioned behind the heat sink 250.

Figure 35 is a detailed perspective view of a portion of the tray 240 that holds the test strips (not shown) as seen from above. The tray 240 includes a front portion having a base 254 and a plurality of discontinuous raised parallel ridge structures 256 with recessed slots 258 for receiving the test strips. The base of the front 254 of the tray 240 is in contact with the 95 degree C heat sink 250. The side walls of the parallel raised ridges 256 at positions 256A and 256B are placed as close as possible to the first and second chambers of the reaction vessel 10 of Figure 1 so as to reduce thermal resistance. The base of the rear of the tray 240 is in contact with a 42 degree C Peltier heat sink as best seen in Figure 34. The portion 256B of the raised ridge for the rear of the

tray is physically isolated from portion 256A for the front of the tray, and portion 256B is in contact with the 42 degree C heat sink so as to keep the second chamber of the reaction vessel in the test strip at the proper temperature.

Still referring to Figure 35 each of the vacuum probes 244 include a rubber gasket 260. When the vacuum probes 244 are lowered by the vacuum probe motor 222 (Figure 32) the gaskets 260 are positioned on the film covering the upper surface of the test strip surrounding the vacuum port in the dual chamber reaction vessel so as to make a tight seal and permit vacuum to be drawn on the second chamber.

Figure 36 is an isolated perspective view of the test strip holder or tray 240 of Figure 35, showing two test strips 19 in accordance with Figure 5 installed in the tray 240. The tray 240 has a plurality of lanes or slots 241 receiving up to 6 test strips 19 for simultaneous processing. Figure 36 shows the heat sinks 242 and 250 for maintaining the respective portions of the tray 240 and ridges 256 at the proper temperature.

Figure 37 is a detailed perspective view of the test strip holder or tray 240 as seen from below. The 95 degree C Peltier heat sink which would be below front portion 254 has been removed in order to better illustrate the rear heat sink 242 beneath the rear portion of the tray 240.

Figure 38 is a block diagram of the electronics and control system of the amplification processing system of Figure 31. The control system is divided into two boards 310 and 311, section A 310 at the top of the diagram devoted to amplification module or station 202 and the other board 311 (section B) devoted to the other module 204. The two boards 310 and 311 are identical and only the top section 310 will be discussed. The two boards 310 and 311 are connected to an amplification station interface board 300.

The interface board 300 communicates with a stand alone personal computer 304 via a high speed data bus 302. The personal computer 304 is a conventional IBM compatible computer with hard disk drive, video monitor, etc. In a preferred embodiment, the stations 202 and 204 are under control by the interface board 300.

The board 310 for station 202 controls the front tray 240 which is maintained at a temperature of 95 degrees C by two Peltier heat sink modules, a pair of fans and a temperature sensor incorporated into the front portion 254 of the tray 240, all of which are conventional. The back of the tray is maintained at a temperature of 42 degrees C by two Peltier modules and a temperature sensor. The movement of the vacuum probes 244 is controlled by the probes motor 222. Position sensors are provided to provide input signals to the tray controller board as to the position of the vacuum probes 244. The tray controller board 310 includes a set of drivers 312 for the active and passive components of the system which receive data from the temperature and position sensors and issue commands to the active compo-

ponents i.e. motors fans Peltier modules etc. The drivers are responsive to commands from the amplification interface board 300. The interface board also issues commands to the vacuum pump for the vacuum subsystem, as shown.

Figure 39 is a diagram of the vacuum subsystem 320 for the amplification processing stations 202 and 204 of Figure 31. The subsystem includes a 1 liter reinforced plastic vacuum tank 210 which is connected via an inlet line 322 to a vacuum pump 323 for generating a vacuum in the tank 210. A vacuum supply line 324 is provided for providing vacuum to a pair of pinch solenoid valves 224 (see Figure 32) via supply lines 324A and 324B. These vacuum supply lines 324A and 324B supply vacuum to a manifold 226 distributing the vacuum to the vacuum probes 244. Note the pointed tips 245 of the vacuum probes 244 for piercing the film or membrane 64 (Figure 11) covering the strip 19. The vacuum system 320 also includes a differential pressure transducer 321 for monitoring the presence of vacuum in the tank 210. The transducer 321 supplies pressure signals to the interface board 300 of Figure 38.

Figure 40 is a representative graph of the thermal cycle profile of the station of Figure 31. As indicated in line 400, after an initial ramp up 402 in the temperature lasting less than a minute, a first temperature T1 is reached (e.g., a denaturation temperature) which is maintained for a predetermined time period, such as 5-10 minutes, at which time a reaction occurs in the first chamber of the reaction vessel. Thereafter, a ramp down of temperature as indicated at 404 occurs and the temperature of the reaction solution in the first chamber of the reaction vessel 10 cools to temperature T2. After a designated amount of time after cooling to temperature T2, e.g., 42 degrees C, a fluid transfer occurs in which the solution in the first chamber is conveyed to the second chamber. Temperature T2 is maintained for an appropriate amount of time for the reaction of interest, such as one hour. At time 406, the temperature is raised rapidly to a temperature T3 of ≥ 65 degrees C to stop the amplification reaction. For a TMA reaction, it is important that the ramp up time from time 406 to time 408 is brief, that is, less than 2 minutes and preferably less than one minute. Preferably, all the ramp up and ramp down of temperatures occur in less than a minute.

Referring now to Figure 41, an alternative and preferred construction for the dual chamber reaction vessel that is suitable for use with the reaction processing station of FIGS. 30-39 and the test strip described previously is illustrated. This embodiment provides a valve means for controlling a connecting conduit linking the first and second chambers together. The valve means was particularly simple to put into effect, both with respect to the construction or design of the reaction vessel and with respect to the external means required for controlling or activating these components.

The valve means includes three components and associated features. First, a connecting conduit is pro-

vided which is flexible that is to say having an internal cross-section of flow which can be reduced simply by the application of external pressure or having a wall which can yield (i.e., deflect inwardly), again by the application of this external pressure. Second, a sealing piece or ball element is disposed within the conduit. This seal piece provides a hermetic seal within the connecting conduit. The seal piece is held in the conduit by the wall of the conduit being pressed against the external surface of the seal piece. Thirdly, the conduit and seal piece are adapted to work together with an external device for constricting the conduit element externally, and set up or positioned in relation to this external device to create a primary or interstitial passage within this conduit piece at the point where the seal piece is located.

Referring now to Figures 41 to 43, a dual chamber reaction vessel 10 in accordance with this embodiment includes a molded body 512 of plastic material. The two flat faces at the front and rear of the body are coated with two films of material (513 and 514 respectively) which seal off the first and second reaction chambers and passages created in the body 512 by the molding process.

Figures 41 and 42 clearly show how the two reaction chambers 502 and 503 are formed, mainly in the body section 512, with one chamber 502 being cylindrical and tapered in shape and the other 503 having a quadrangular cross-section. These two chambers are joined together by a connecting flexible conduit 504 similar to a siphon. One end of the conduit 504 is in communication via a front orifice 510 to the lower part of the chamber 502. The other end of the conduit 504 has a rear orifice 511 set at the top of the other chamber 503, and passing via a vertical conduit portion 505 which is described in further detail below.

A means to control, in particular to open, the connection conduit 504 described above is provided in the conduit portion 505. In particular, an external device 508 is provided for constricting the conduit portion 505. The external device 508 is inserted into the reaction vessel 10 from the side to which the equipment or control system is connected to the conduit portion 505, for example from above the test strip when the reaction vessel is positioned in a test strip and installed in the processing station of FIGS. 31-39.

As shown in FIGS. 41-44, in a first embodiment, the conduit portion 505 is flexible, meaning that its internal cross-section can be reduced by applying an external pressure, such as pressure applied peripherally or centripetally. As with the body 512, this conduit piece 505 is made from plastic material, such as low density polyethylene for example.

A substantially rigid seal piece 506, consisting of a ball of glass or metal, is held in the interior 505a of the conduit portion 505. The seal piece 506 is held in place solely by the force of wall 507 of the conduit portion being pressed against the external surface of the seal piece 506. The seal piece 506 and the internal cross-

section of the inside of the conduit portion 505a are both arranged so that the position for the seal piece 506 ensures that the seal piece provides a tight seal on the inside of the conduit portion 505a.

The conduit portion 505 consists of two parts. The first part 505b has a relatively narrow internal cross-section in which the seal piece 506 is held by the pressing action. The second part 505c has a relatively wide internal cross-section in which the seal piece 506 cannot be held by the pressing action and therefore falls to the bottom of the connecting conduit 504.

As stated previously, an external device 508 is provided on the automatic analysis apparatus side (i.e., above the dual chamber reaction vessel) to constrict the conduit portion 505. This external device is represented schematically in Figures 43 and 44 by two arms (581 and 582) fitted with pinch bars (581a and 582a respectively). Openings 521 and 522 are provided in the body 512 on either side of the conduit portion 505 to allow the two arms 581 and 582 to move freely (upwards and downwards, for example) and into a position for cooperating with the ball or seal piece 506. For example, and with reference to FIG. 33, each of the vacuum probe tools 244 may incorporate arm elements 581 and 582 which cooperate with the seal piece 506 to open the conduit 505 when they (tools 244) are lowered down onto the test strip.

As shown in Figure 44, the external constriction device 508 is positioned to move along the conduit portion 505 and push the seal piece 506 from the first part of the conduit portion 505b to the second part 505c without coming into contact with it. This allows the seal piece 506 to fall to the bottom of the conduit portion and free or open the passage in the conduit piece.

Two external stops 505d (Figure 41) are provided on the outside of the conduit portion to stop movement, for example downward movement, of the arms 81 and 82.

Referring now to Figure 45, in a second variation of the embodiment of Figure 41, the wall 507 of the conduit device 507 can yield, again by the application of external pressure, for example pressure applied peripherally or centripetally, when the relatively hard seal piece 506 comes into contact with it. In this case, the constricting device 508 is set up so that when it is in its lowered position, it makes an impression of the seal piece 506 in the wall 507 to create a lasting internal imprint 509. When the external constricting device 508 releases this pressure an interstitial passage is created after the constricting device 508 has acted between the seal piece and the wall 507. This interstitial passage enables or releases flow through the connecting conduit 504. The dotted line to the left of Figure 45 shows the ball 506 in the position it is held in conduit 505, with the solid line at the right of the illustration showing the imprint made by the action of the constricting device 508.

Another representative example of how the dual chamber reactions vessels of this disclosure may be

loaded with fluid sample and of how the fluid samples may be transferred from one chamber to another will be described in conjunction with Figure 46 and 47A-47E.

As shown on Figure 46, a dual chamber reaction

vessel 600 comprising a body 612 made for example from molded plastic material. The vessel 600 includes a first chamber 602, made from plastic material, in communication with the outside via a conduit 604, with the closure and/or opening of this conduit controlled by a system, such as a valve, which is represented schematically by reference number 606. One the other side of the control system 606, this first conduit is in communication with an angled sampling conduit 608, which is described in further detail below. The vessel also includes a second chamber 603 in communication with the first chamber 602 only, via a second connecting conduit 605, which also has closing and/or opening operations controlled by a system, such as a valve, which is represented by the general reference number 607. The valve 607 and conduit 605 may, for example, take the form of the conduit and ball valve described previously, the elastomeric thimble valve and conduit described earlier, or the spike structure that is operated to pierce a membrane and described above.

The component of the type illustrated in Figure 46 is generally operated within a gaseous external environment, at a reference pressure, hereinafter termed high pressure, for example atmospheric pressure.

Further, the first and second chambers are loaded with reagent and enzymes in the manner described previously at the time of manufacture.

As an example, a first chemical or biochemical reaction takes place in the first chamber 602, causing this chamber to contain a first reagent, and the reagent product obtained in chamber 602 is subjected to a further reaction in chamber 603, causing chamber 603 to contain a reagent or product which is different from the reagent originally contained in chamber 602.

A process is illustrated in Figures 47A-47F whereby

a liquid sample 611 contained in an external container, a test tube 610 for example, is transferred into the first chamber 602 and then into the second chamber 603. The second chamber 602 is originally under high pressure, with the second conduit 605 being closed, and chambers 602 and 603 are isolated from each other. With the first conduit 604 being open, the first chamber 602 is in communication with the external environment and is therefore under high pressure HP (see Fig. 47A).

The first chamber 602 is brought down to a reduced pressure by the first conduit 604, i.e., a pressure being lower than the pressure termed low pressure which is described in further detail below, this is achieved by means of an arrangement such as connecting the first conduit 604 to an evacuation device or pump 609 (see Fig 47B). The first conduit 604 is then closed

The free end of the angled tube 608 is immersed in the liquid 611 to be transferred contained in container 610. The first conduit 604 is in communication with the

liquid at an immersed level via this angled tube 608 with the liquid being located in the gaseous external environment and hence subjected to high pressure. The first conduit is then opened, causing the liquid to be transferred into the first chamber 602 via the first conduit 604 (see Figure 47C). Finally, the pressure in the first chamber 602 becomes established at a value termed reduced pressure (RP) which is greater than the pressure termed low pressure mentioned above, although remaining lower than the pressure termed as high pressure.

The first conduit 604 is closed to produce the situation shown in Figure 47D. The second conduit 605 is closed and the two chambers 602 and 603 are isolated from each other, with the second chamber 603 being at high pressure with the first conduit 604 closed, and the second chamber 602 being isolated from the outside and partially filled with the liquid previously transferred, whilst being at reduced pressure.

The second conduit 605 is opened (i.e., by opening the valve 607), causing the pressure in the two chambers 602 and 603 to become balanced at a pressure termed intermediate pressure (IP) which is between the high and reduced pressure values (see Figure 47E).

The first conduit 604 is then opened, causing the first chamber 602 to be in communication with the external high pressure environment, and the liquid is transferred from the first chamber 602 to the second chamber 603 via the second conduit 605 (see Figure 47F). The pressure in the two chambers finally reaches the high pressure value. The first conduit 604 can be sealed permanently when the entire process has been completed. The reaction can then proceed in chamber 603. Of course, chambers 602 and 603 may be maintained at separate temperatures in accordance with the principles of the invention set forth above.

While presently preferred embodiments of the invention have been described herein, persons of skill in the art will appreciate that various modifications and changes may be made without departure from the true scope and spirit of the invention. For example, the novel reaction vessels and test strips can be used in other reactions besides isothermal amplification reactions such as TMA. The invention is believed to be suitable for many isothermal reactions, other enzymatic reactions, and reactions requiring differential heating and containment. For example, the reference to "denaturation and cooling", while specifically applicable to the TMA reaction, can be considered only one possible species of a heat differential step. Further, the spatial and temperature isolation of the amplification enzyme in the second chamber is considered one example of spatial isolation of a heat labile reagent. The invention is fully capable of being used in other types of reactions besides TMA reactions. This true scope and spirit is defined by the claims to be interpreted in light of the foregoing

Claims

1. A dual chamber reaction vessel for a nucleic acid amplification reaction characterised in that it comprises

a first chamber for receiving a fluid sample, the said first chamber being loaded with one or more amplification reagents.

a second chamber physically isolated from the said first chamber;

one or more enzymes for the said reaction either in the said second chamber or in fluid communication with the said second chamber;

and

a fluid channel connecting the said first chamber to the said second chamber.

2. A vessel as claimed in claim 1 wherein it further comprises a means for selectively opening the said fluid channel to allow a fluid to pass from the said first chamber into the said second chamber.

3. A vessel as claimed in claim 1 or claim 2 wherein the said means for selectively opening the said fluid channel comprises a breakable seal, preferably the said means for selectively opening the said fluid channel comprising a means for creating fluid pressure in the said sample fluid so as to break the said seal and enable fluid to flow from the said first chamber through the said fluid channel into the said second chamber, or the said means for selectively opening the said fluid channel comprising a plunger reciprocable within the said vessel from a first position to a second position, the said plunger in the said second position being operable to cut the said seal and thereby open the said fluid channel; or the said means for selectively opening the said fluid channel comprising a valve, preferably a thimble valve.

4. A vessel as claimed in any of claims 1 to 3 wherein it further comprises a vacuum port in fluid communication with the said second chamber, such that the application of vacuum to the said vacuum port draws the said fluid sample from the said first chamber into the said second chamber.

5. A dual chamber reaction vessel characterised in that it comprises:

a first chamber and a second chamber joined together via a connecting conduit,

and

a valve means for opening the said conduit comprising

(a) a flexible conduit portion linking the said

- first and second chambers having a wall portion

(b) a substantially rigid seal piece disposed within the said flexible conduit: the said seal piece providing a tight seal within the said conduit portion and being held in the conduit by the said wall of the conduit portion pressed against the said seal piece:

and

(c) an external device for constricting the said conduit portion: the said conduit piece cooperating with the said external device for constricting the said conduit portion. the said conduit portion being positioned in relation to the said external device such that relative motion between the said conduit portion and the said external device causes the said constricting device to act on the said seal piece to open the said conduit portion and create a passage within the said conduit portion at the point where the said seal piece is located.

6. A vessel as claimed in claim 5 wherein the said seal piece comprises a ball.

7. A vessel as claimed in claim 5 or claim 6 wherein the said conduit portion. which is preferably made from a flexible plastic material, further comprises an internal section which may be reduced by the application of an external pressure and consists of a first portion having a relatively narrow internal cross-section in which the seal piece is held by the wall of the said conduit portion. and a second portion with a relatively wide cross-section in which the said seal piece cannot be held by the said wall, the said first and second portions being oriented such that the said external constriction device may be moved along the said conduit portion to push the said seal piece from the said first portion to the said second portion. and, optionally, further comprising at least one external stop incorporated on the outside of the conduit portion to halt the movement of the constriction device into the said dual chamber reaction vessel

8. A vessel as claimed in any of claims 5 to 7 wherein the said conduit piece further comprises a relatively yielding wall and the external constriction device is operative to make an impression of the shape of the outside of the seal piece in the said wall to create an imprint on the inside of the said wall to allow an interstitial flow between the said seal piece and the said wall after action of the constriction device

9. A vessel as claimed in any of claims 5 to 8 wherein the said first and second reaction vessel and the said conduit portion are made from a single mould-

10. A vessel as claimed in any of claims 5 to 9 wherein the said external constriction device comprises a pair of arms. the said arms cooperating with the said seal piece to move the said seal piece from a first location in the said conduit portion to a second location in the said conduit portion when the said pair of arms are moved relative to the said dual chamber reaction vessel.

11. A two-piece disposable reaction vessel characterised in that it comprises:

a first piece comprising a first chamber containing an amplification reagent:

and

a second piece comprising a second chamber containing an amplification enzyme:

the said first and second pieces being constructed so as to permit the said first and second pieces to be securely joined into a dual chamber reaction vessel such that a fluid sample in the said first chamber may pass into the said second chamber.

12. A reaction vessel for a nucleic acid amplification reaction characterised in that it comprises:

an amplification well:

a channel separated from the said amplification well by a heat and moisture barrier:

a carrier in the said channel carrying an amplification enzyme:

the said carrier being moveable within the said channel such that the said carrier may be moved through the said heat and moisture barrier to deliver the said enzyme to the said amplification well.

13. A nucleic acid amplification station for a test strip comprising a dual chamber reaction vessel comprising a first chamber and a second chamber. characterised in that the station comprises:

a tray for at least one test strip. the said tray comprising a first portion and a second portion positioned adjacent to the said first and second chambers of the said dual chamber reaction vessel. respectively:

a temperature control subsystem for the said tray maintaining the said first and second portions of the said tray at first and second different amplification reaction temperatures so as to maintain the said first and second chambers at the said first and second amplification reaction temperatures respectively

a fluid conduit opening mechanism for opening

- a fluid conduit in the said dual chamber reaction vessel to establish fluid communication between the said first chamber and the said second chamber
and, optionally.
- a vacuum subsystem comprising a vacuum probe, the said test strip and vacuum probe being mutually reciprocable and the said vacuum probe cooperating with reaction wells in the said test strip for transferring a fluid sample from the said first chamber to the said second chamber via the said fluid conduit.
14. A station as claimed in claim 13 wherein the said fluid conduit opening mechanism comprises a pin for the said test strip reciprocable with the said vacuum probe relative to the said test strip.
15. A station as claimed in claim 13 or claim 14 wherein the said vacuum probe comprises a tip portion and the said fluid conduit opening mechanism comprises the said tip portion of the said vacuum probe.
16. A station as claimed in any of claims 13 to 15 wherein in the said temperature control subsystem further comprises a first heat sink for heating the said first portion of the said test strip to the said first temperature and a second heat sink, isolated from the said first heat sink, for maintaining the said second portion of the said test strip at the said second temperature.
17. A station as claimed in any of claims 13 to 16 wherein in the said tray comprises a base and a plurality of raised ridges defining slots for receiving a plurality of test strips, preferably the said raised ridges being discontinuous, with a first portion of the said raised ridges in contact with a first heat sink and a second portion of the said raised ridges in contact with a second heat sink.
18. An amplification processing station characterised in that it comprises a dual chamber reaction vessel as claimed in claim 10, the said arms reciprocating from a first position to a second position and the said arms, in the said second position, opening the said conduit portion
19. A test strip characterised in that it comprises a reaction vessel as claimed in any of claims 1 to 12 and optionally, an optical cuvette for conducting an optical analysis of a sample
20. A test strip for a nucleic acid amplification reaction characterised in that it comprises a body portion defining a plurality of wells arranged in a row and having a first end and a second end the said second end having a cuvette for conducting an optical anal-
- ysis of a sample and an aperture provided in the said body portion adjacent to said first end of said test strip for receiving a disposable amplification reaction vessel, preferably a vessel as claimed in any of claims 1 to 12
21. A method for conducting a nucleic acid amplification reaction characterised in that it comprises:
- providing a dual chamber reaction vessel comprising first and second chambers capable of being placed in fluid communication, the said dual chamber reaction vessel being loaded with one or more amplification reagents in the said first chamber and one or more amplification enzymes in the said second chamber;
- sealing the said first and second chambers with the said amplification reagent(s) and amplification enzyme(s) from the environment with a membrane;
- and, at the time of use of the said dual chamber reaction vessel,
- piercing the said membrane with an implement and loading a sample into the said first chamber;
- heating the said first chamber and the said sample to a first relatively high temperature, while maintaining the said second chamber at a second relatively low temperature;
- cooling the said first chamber and a solution of the said sample and the said amplification reagent(s) from the said first relatively high temperature;
- either passing the said solution from the said first chamber to the said second chamber, or introducing the contents of the said second chamber into the said first chamber;
- and
- amplifying the said solution either in the said second chamber or in the said first chamber by means of the said amplification enzyme;
- and, optionally,
- applying vacuum to the said second chamber so as to draw the said solution through the said fluid channel from the said first chamber to the said second chamber, if the said amplification reaction is to occur in the said second chamber.
22. A method for conducting a nucleic acid amplification reaction characterised in that it comprises:
- providing a reaction vessel comprising a first amplification chamber and a second chamber separated from the said amplification chamber by a heat and moisture barrier;
- loading one or more amplification reagents into the said amplification chamber and one or more amplification enzymes into the said second

chamber
loading a sample into the said amplification chamber
heating the said first chamber and the said sample to a first relatively high temperature greater than or equal to 65 degrees C. while maintaining the said enzyme in the said second chamber at a second relatively low temperature: 5
cooling the said first chamber and a solution of the said sample and the said amplification reagent(s): 10
introducing the said amplification enzyme(s) into the said amplification chamber by forcing the said enzyme(s) through the said heat and moisture barrier into the said amplification chamber: 15
and
amplifying the said solution in the said amplification chamber. 20

23. A process for transferring a liquid within a reaction vessel comprising a first chamber, which communicates with the outside by means of a first conduit, and a second chamber, which communicates with the first chamber by means of a second connecting conduit, in the presence of an external gaseous environment at a pressure termed high pressure characterised in that it comprises: 25

- (a) isolating the said first and second chambers from each other by closing the said second connecting conduit, the said first and second chambers being at the said high pressure: 30
- (b) reducing the pressure in the said first chamber to a low pressure lower than the said high pressure, the said second chamber being maintained at the said high pressure: 35
- (c) introducing a fluid sample into the said first chamber via the said first conduit, the said first conduit being placed in fluid communication with the said fluid sample, and thereafter closing the said first conduit: 40
- (d) opening the said conduit to cause the pressure in the two chambers to become balanced at an intermediate pressure having a value between the said high and low pressures: 45
- (e) opening the said first conduit to cause the said first chamber to be in communication with the outside at high pressure: 50
- and
- (f) transferring the said liquid from the first chamber to the second chamber via the second conduit with the pressure in the two chambers finally reaching the said high pressure 55

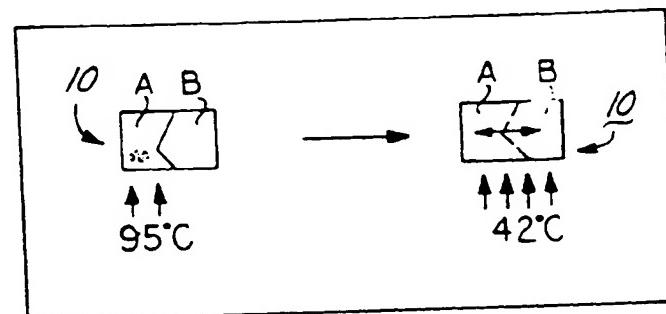


FIG.1

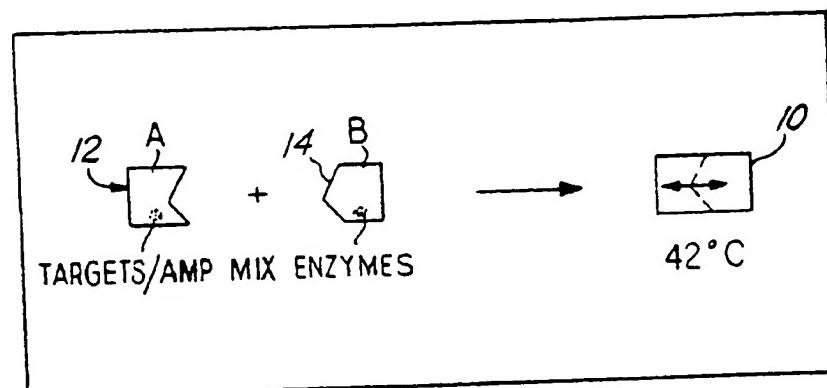


FIG.2

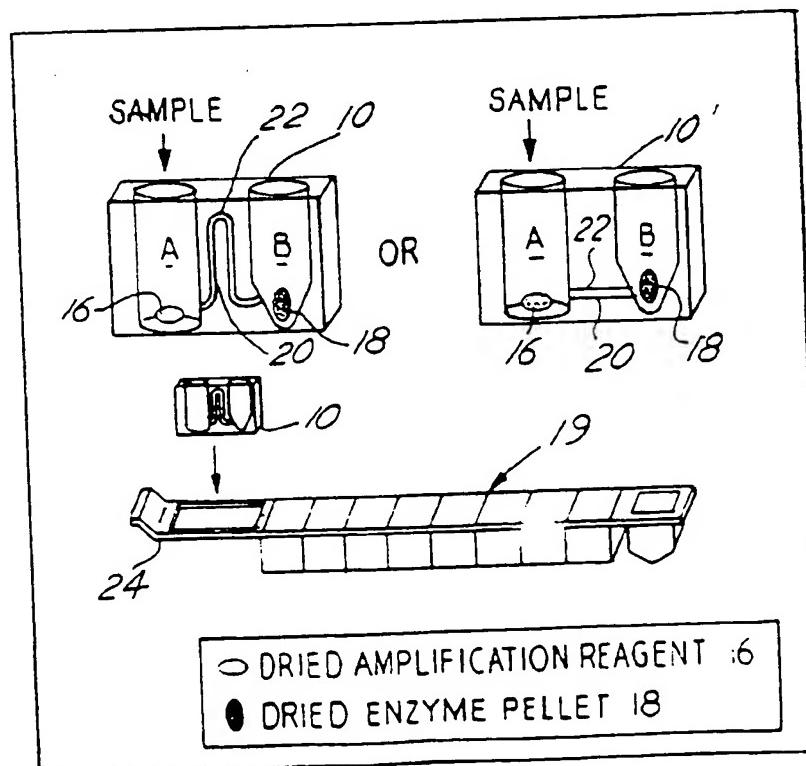
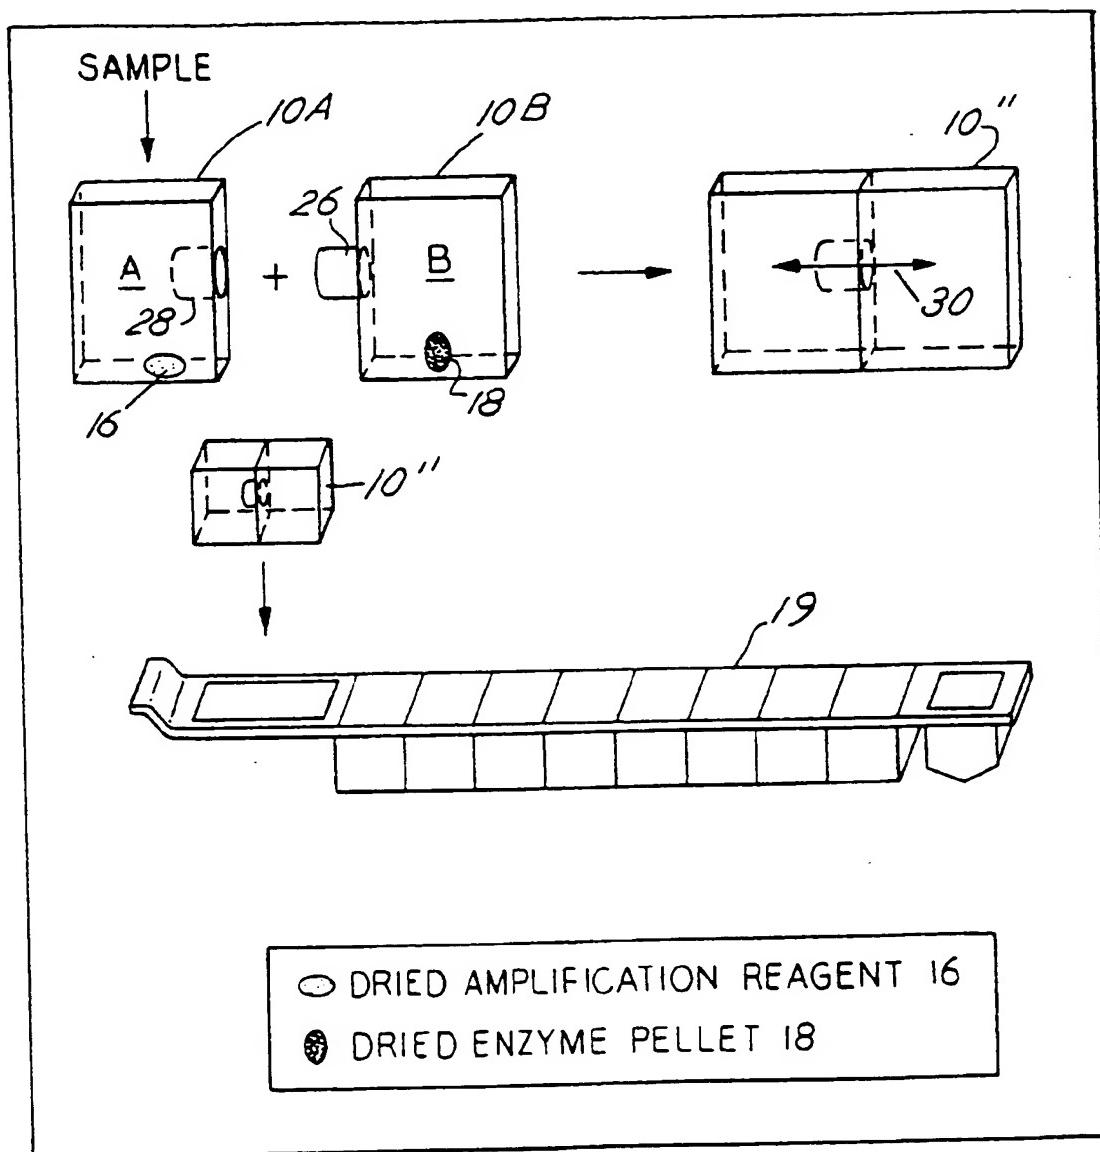


FIG.3

FIG.4



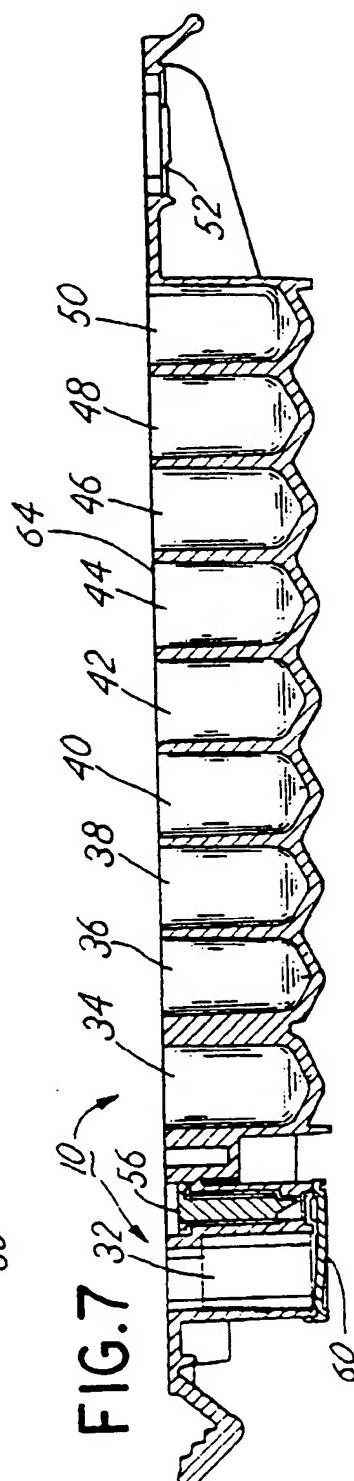
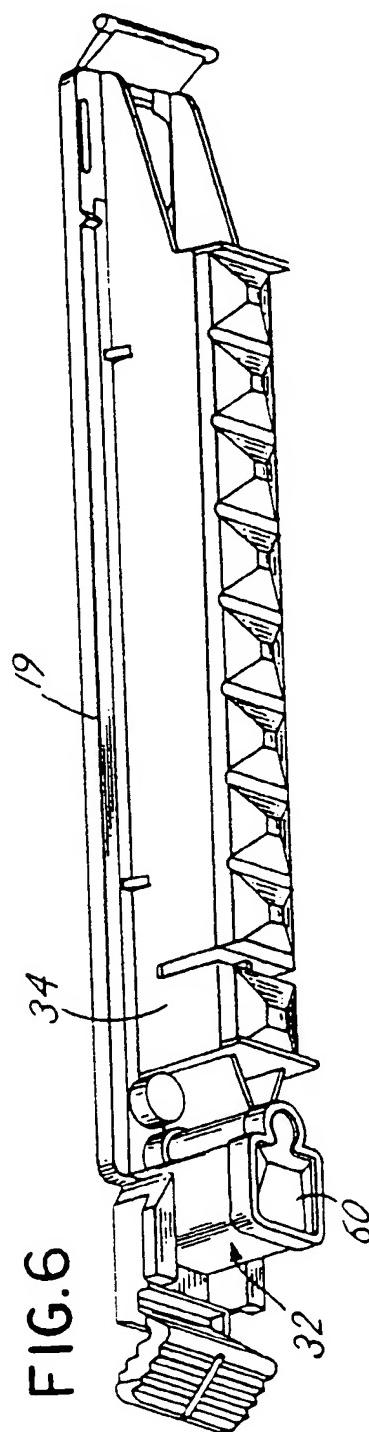
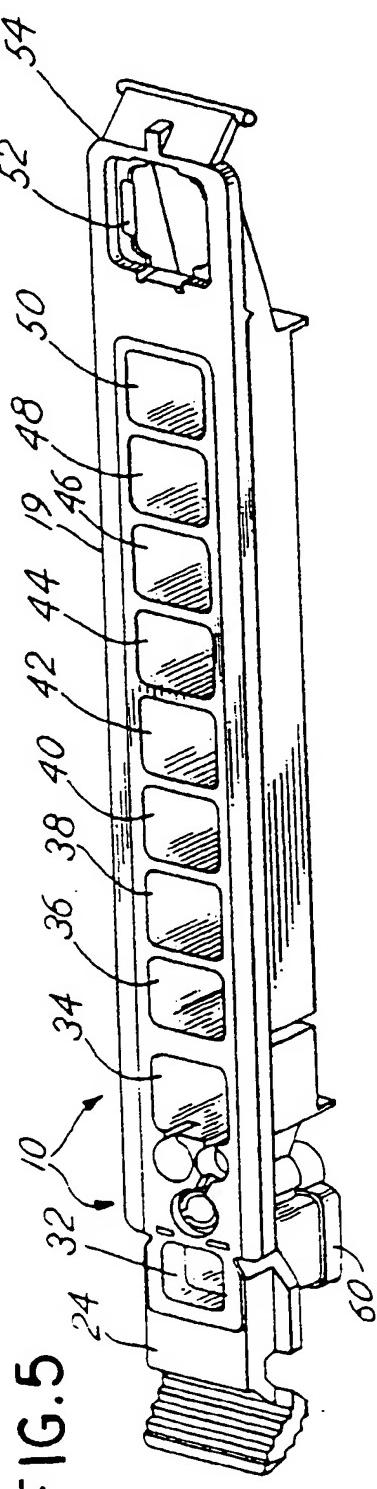


FIG. 8

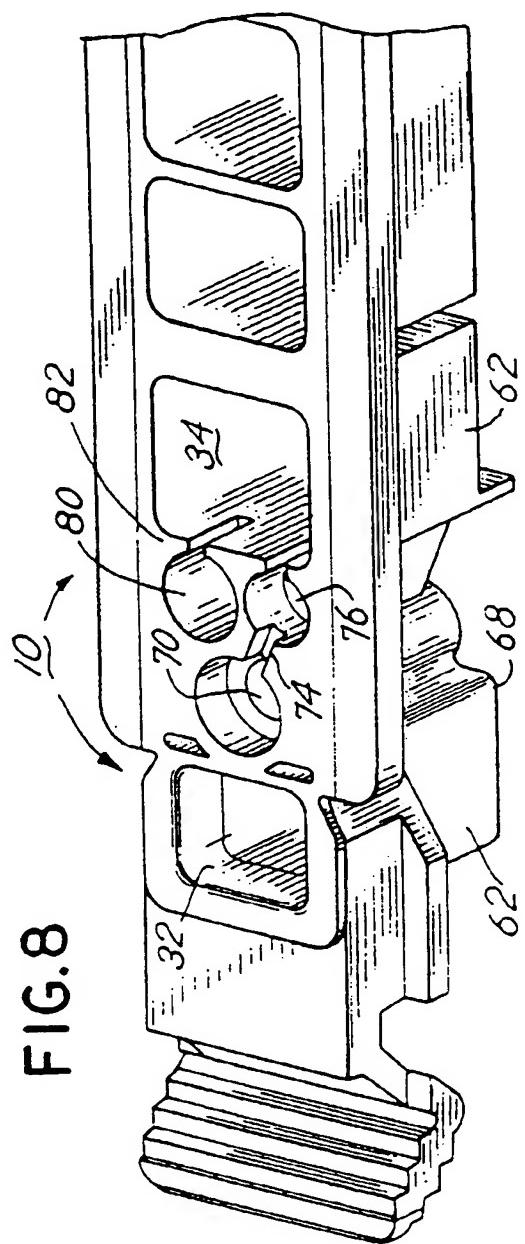


FIG. 9

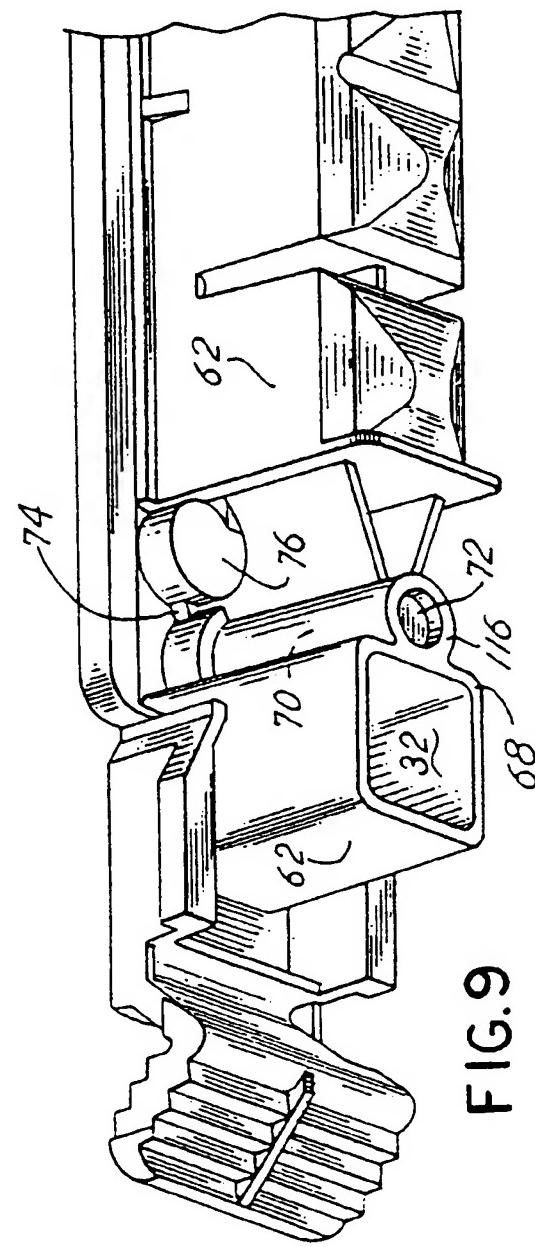


FIG.10

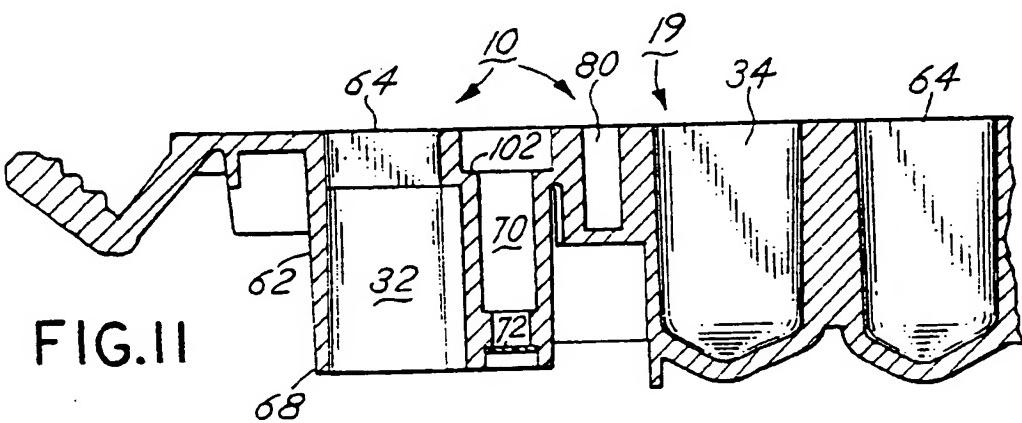
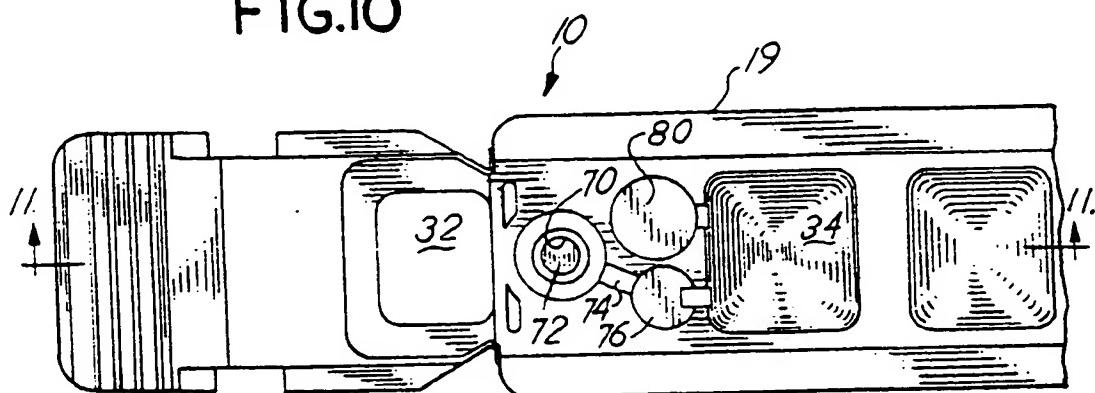


FIG.11

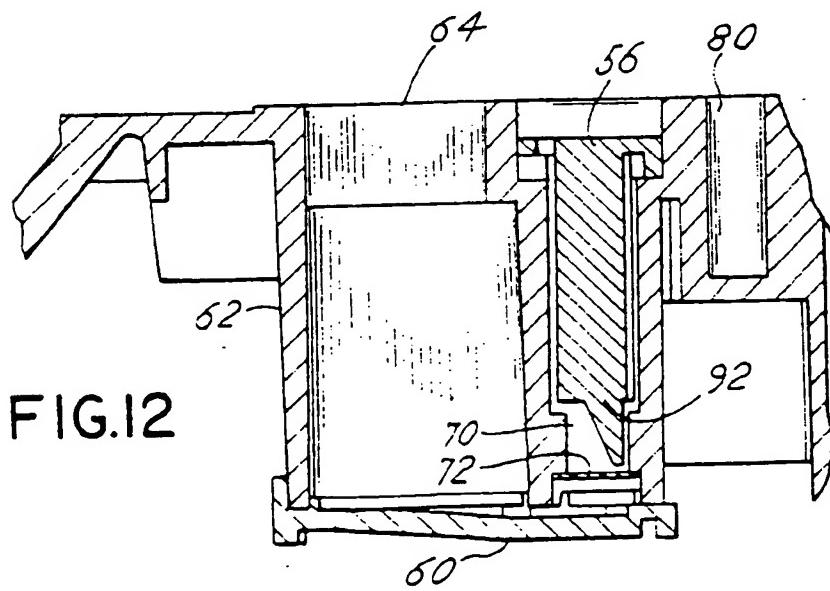


FIG.12

FIG.13

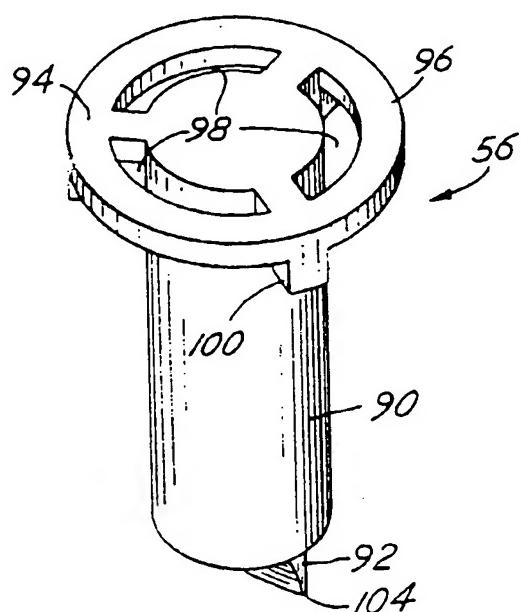


FIG.14

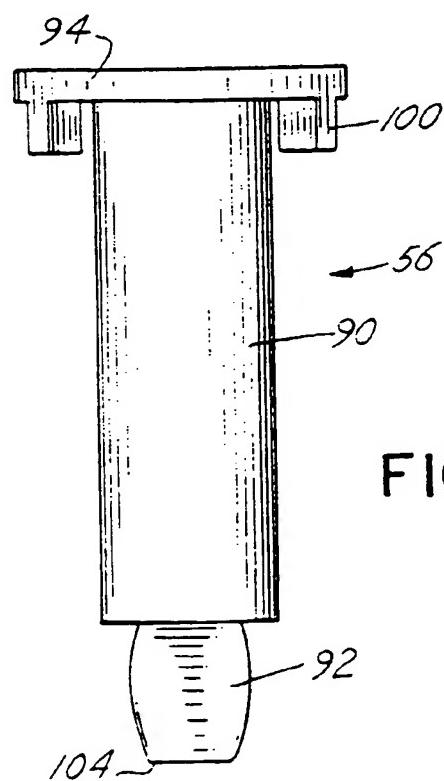
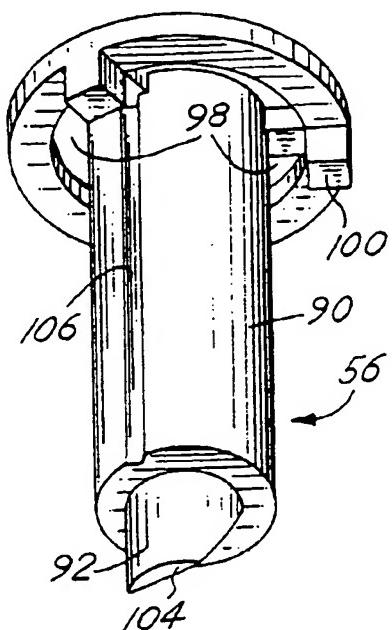


FIG.15

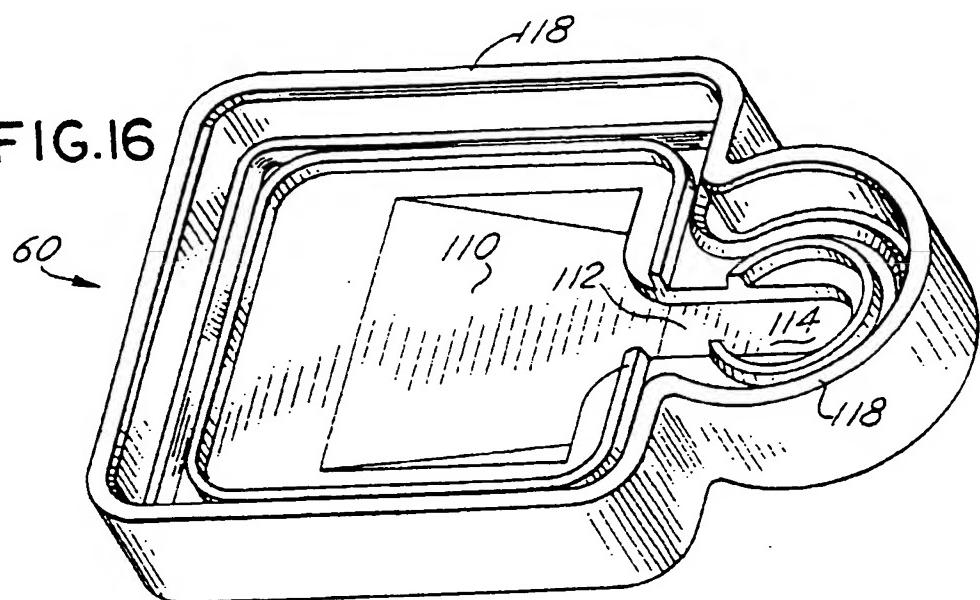
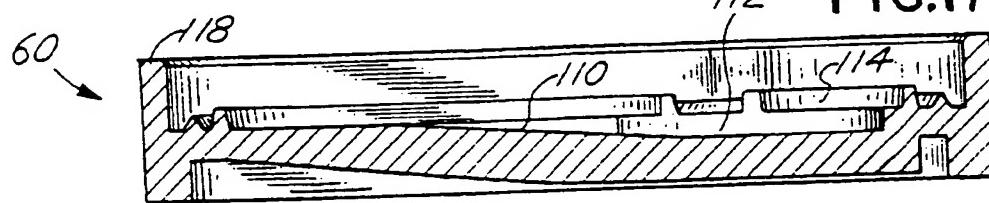
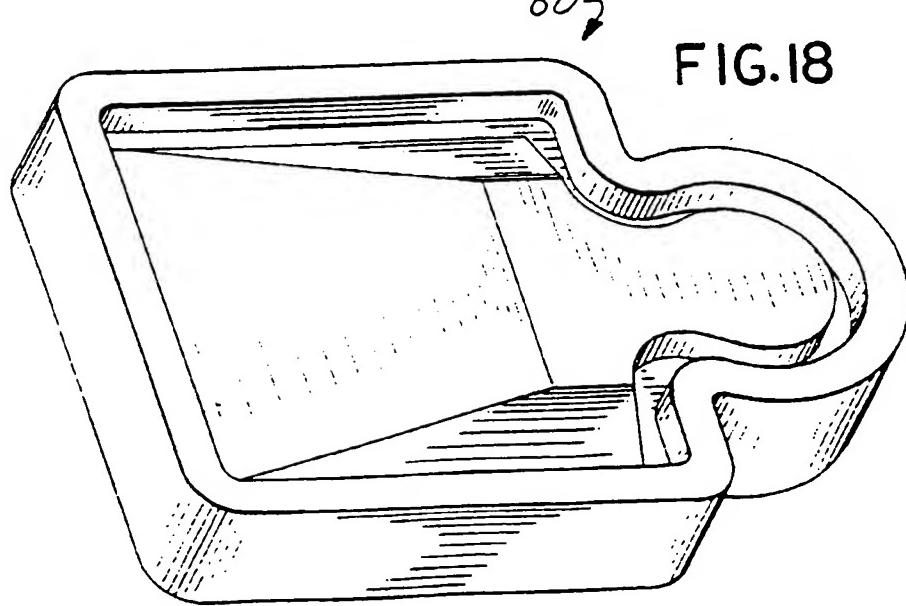
FIG.16**FIG.17****FIG.18**

FIG.19

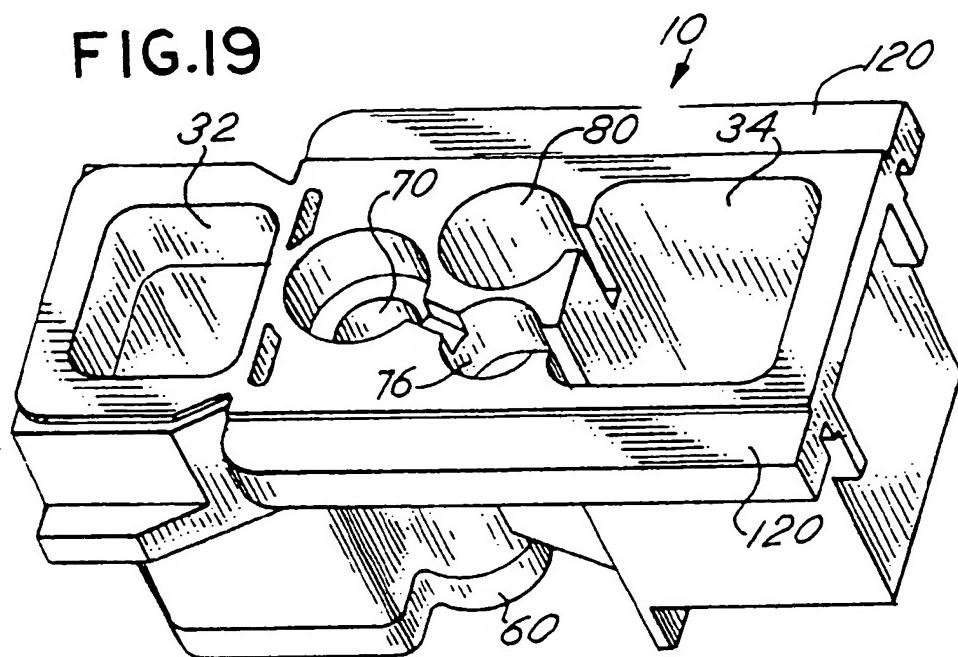
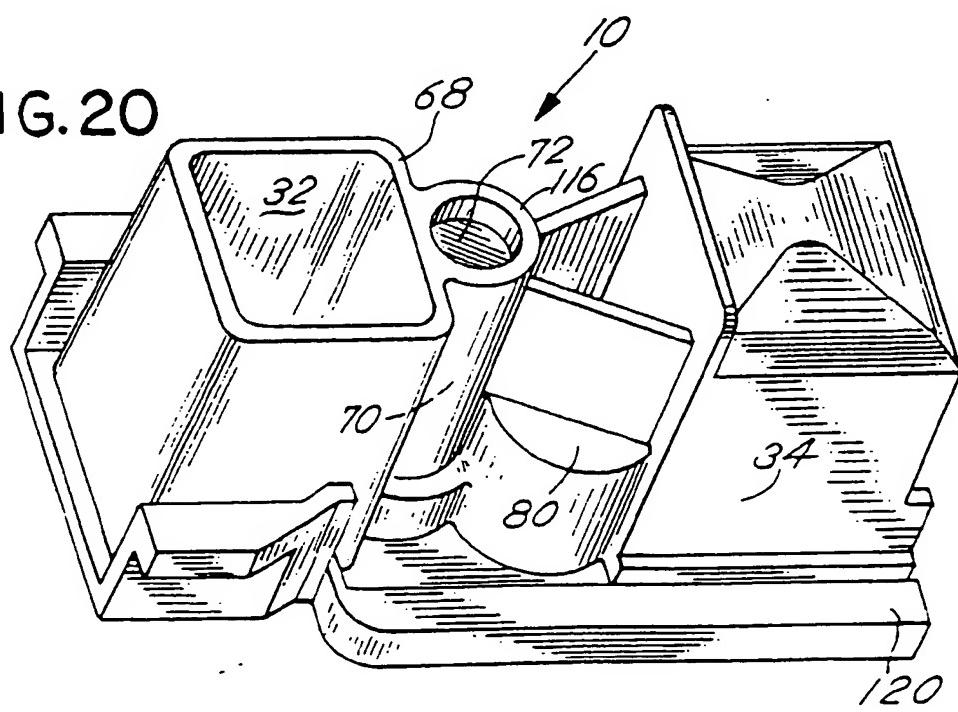


FIG.20



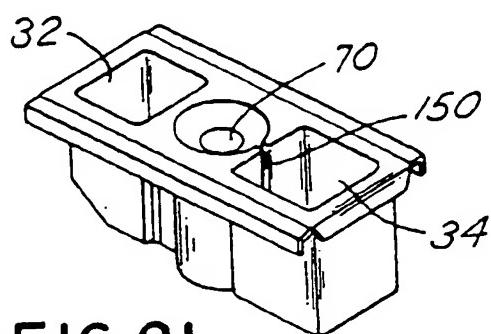


FIG. 21

FIG. 24

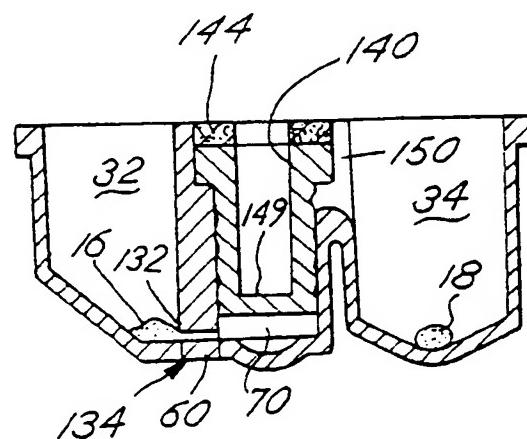
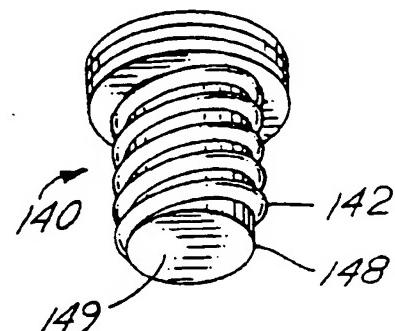


FIG. 22

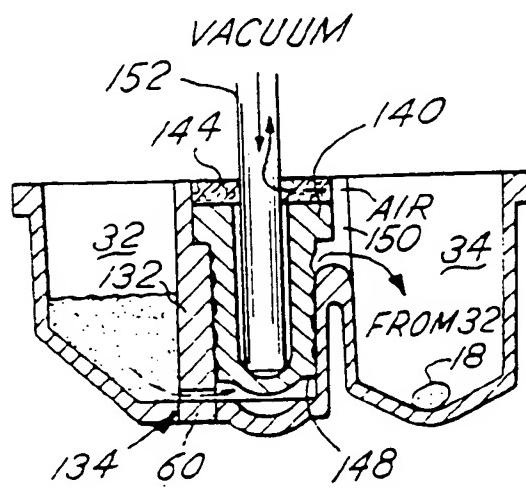
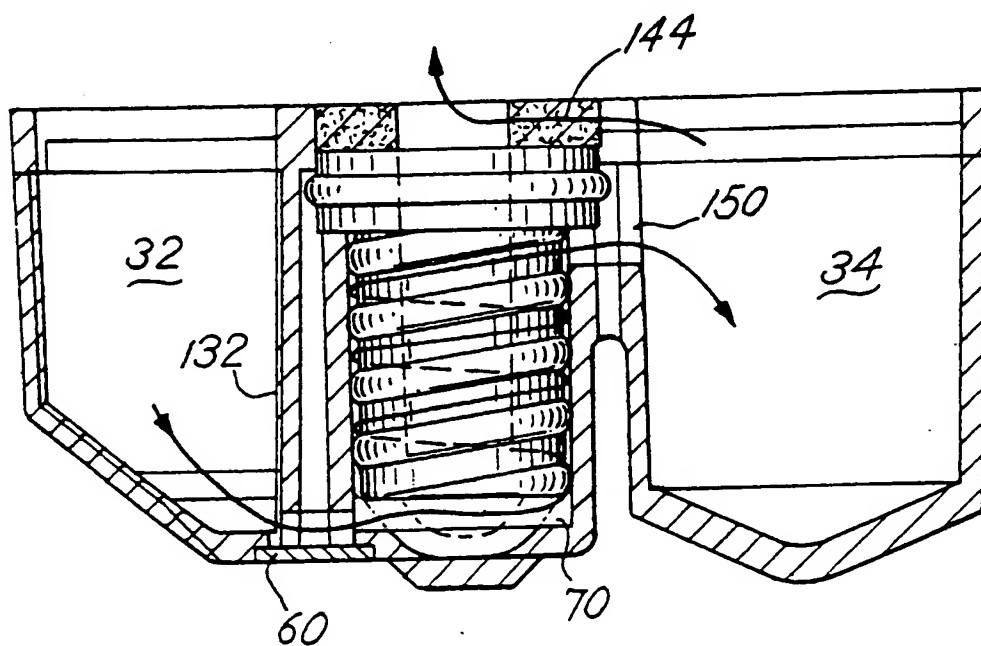


FIG. 23

FIG.25



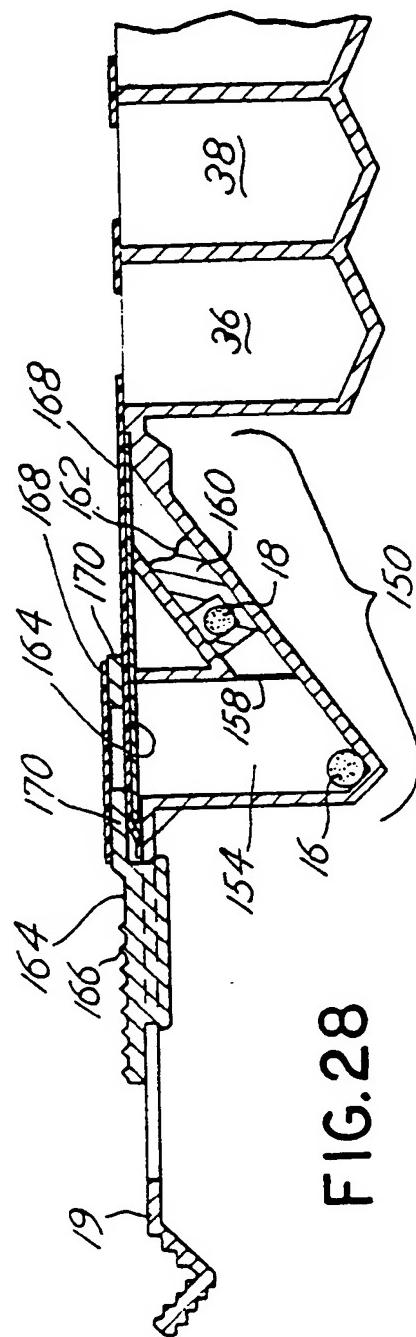
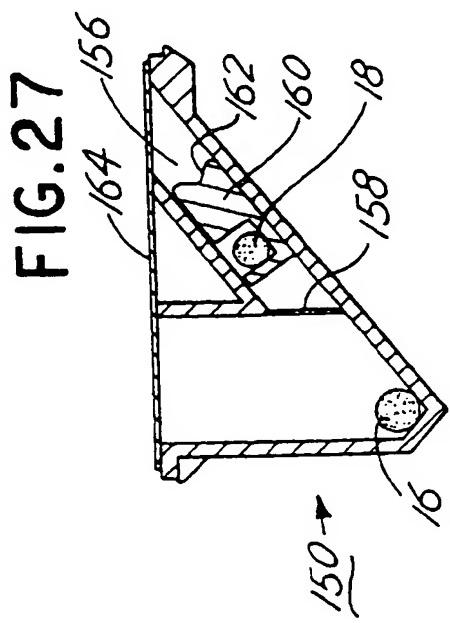
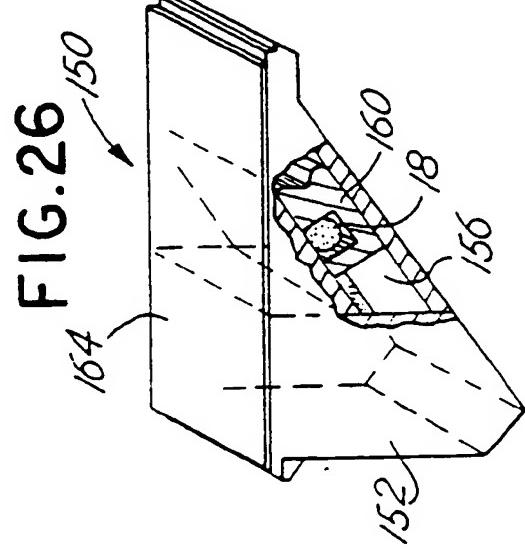


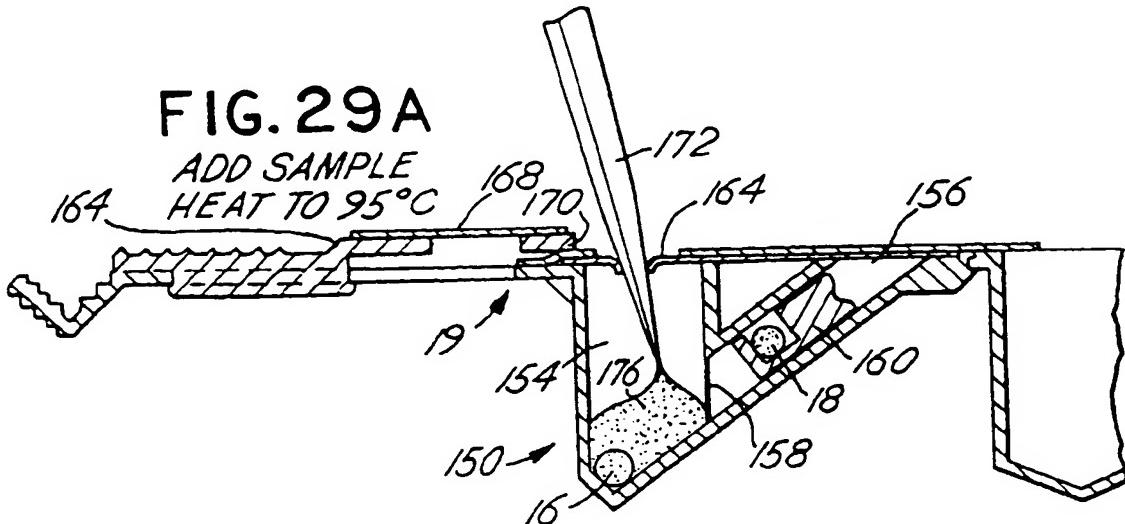
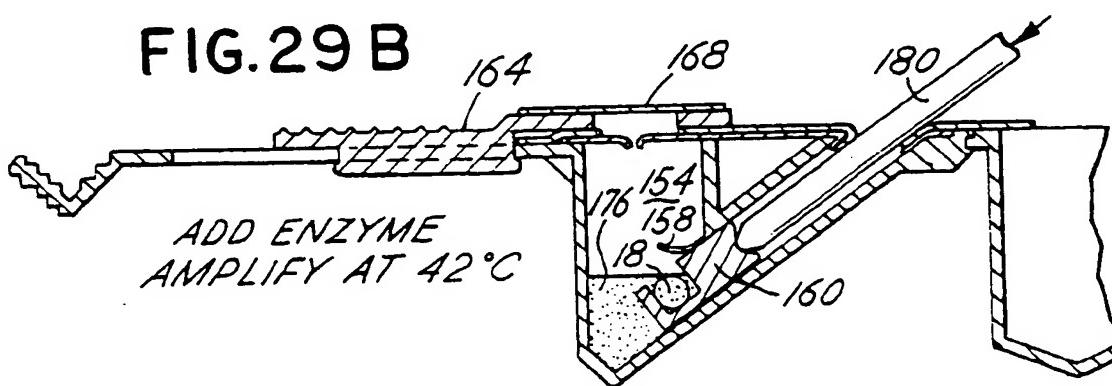
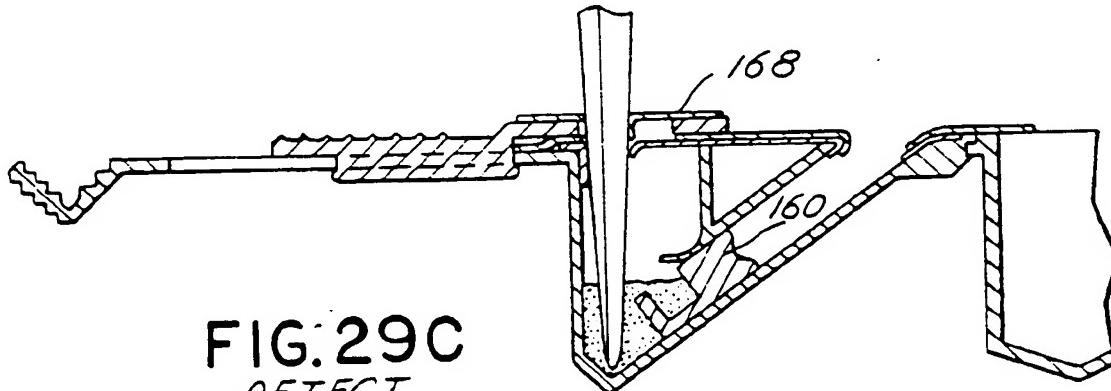
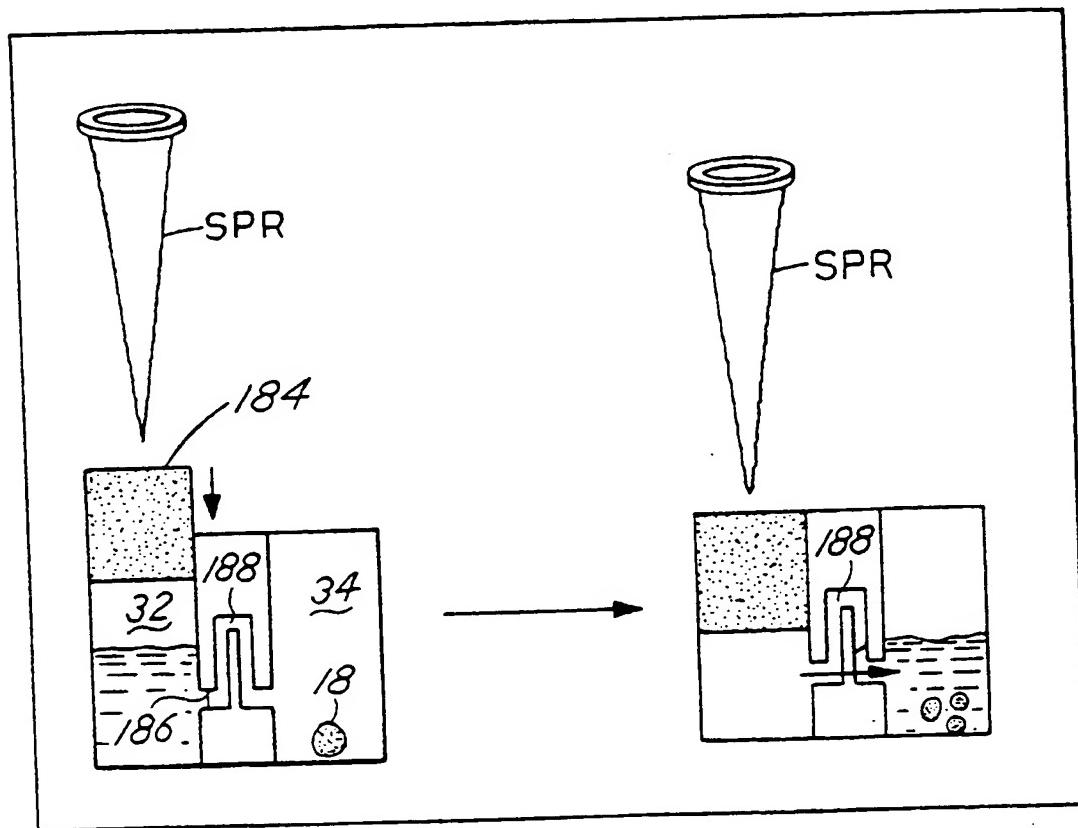
FIG. 29A**FIG. 29 B****FIG. 29C
DETECT**

FIG.30



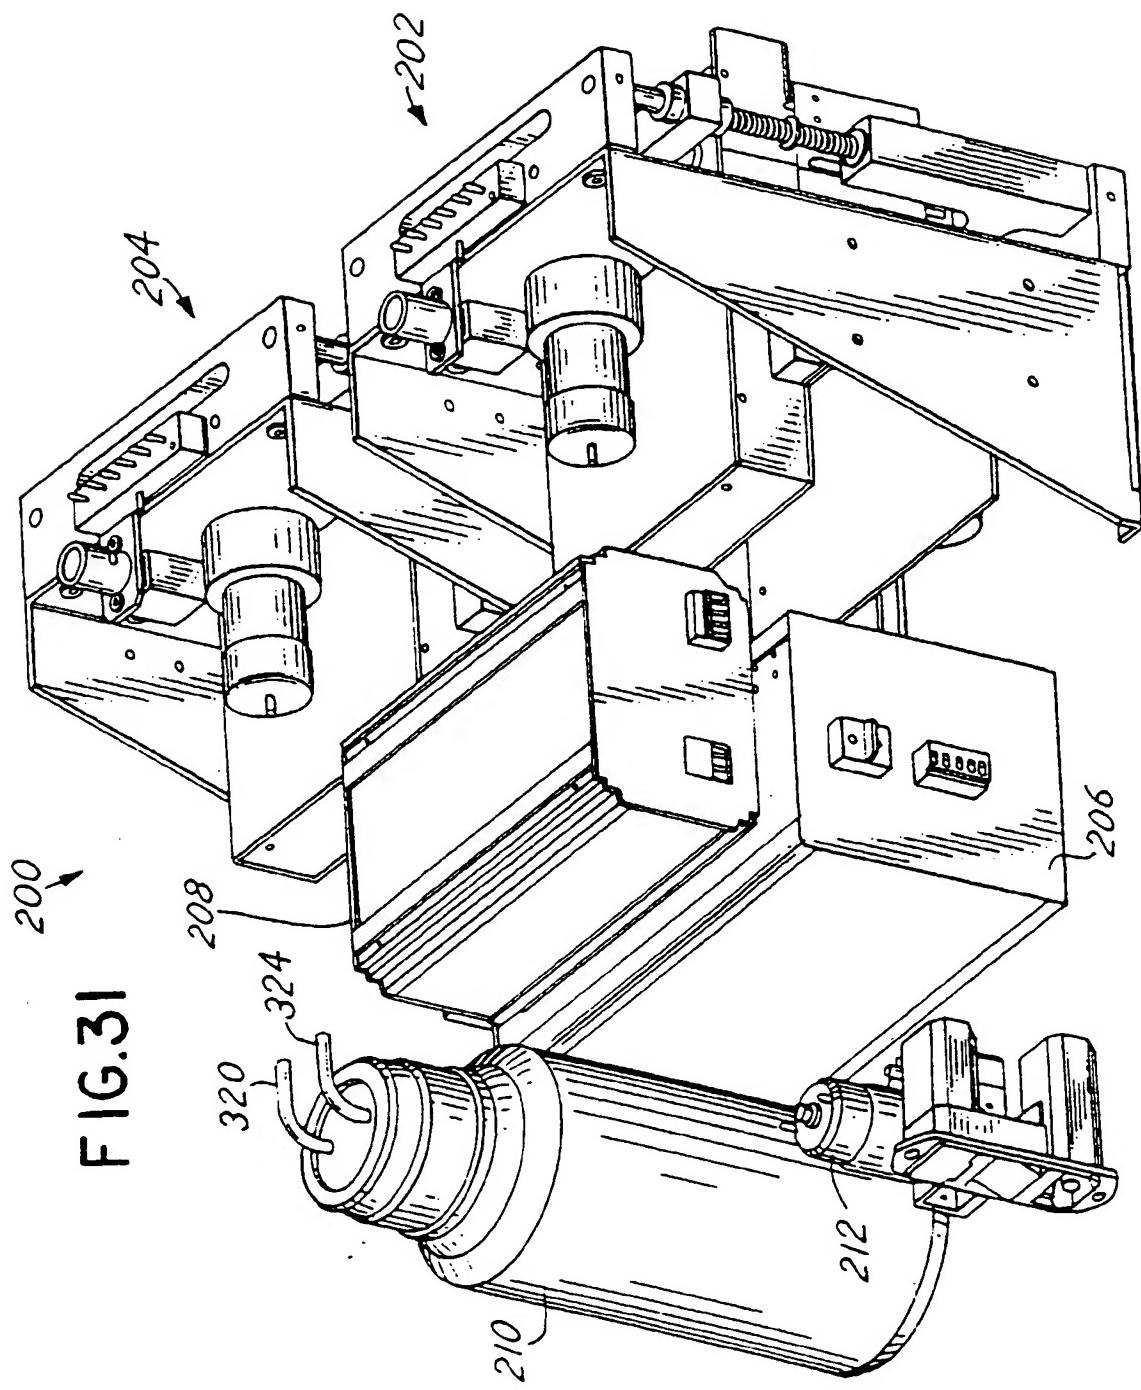


FIG. 31

FIG.32

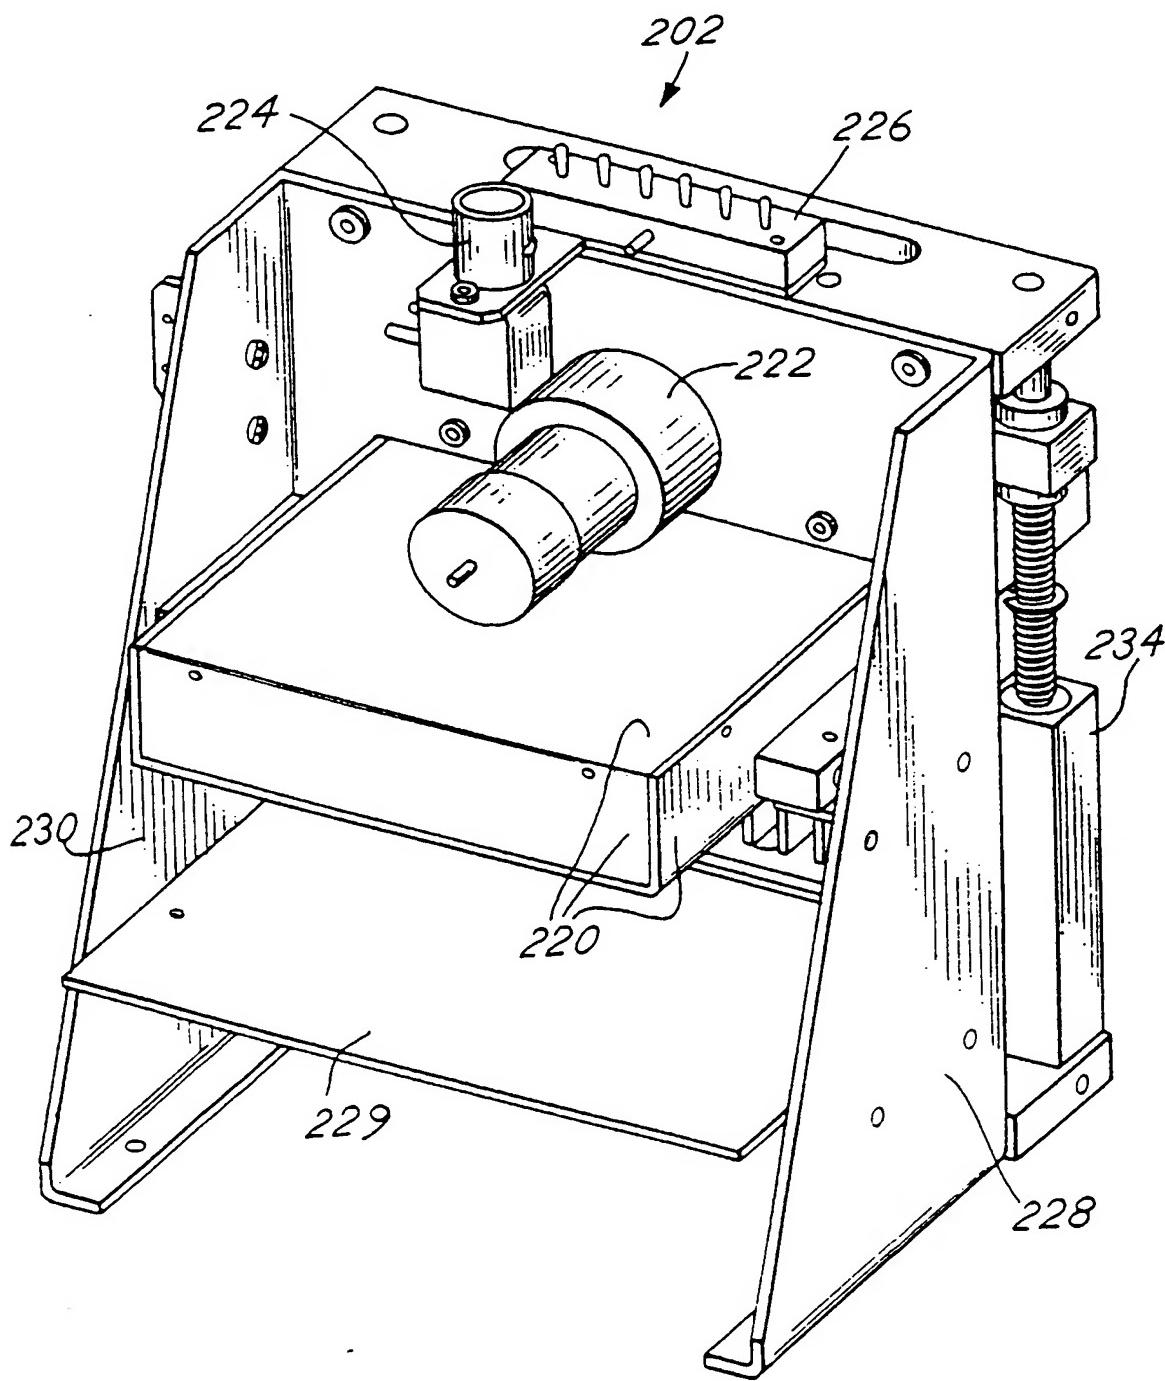


FIG. 33

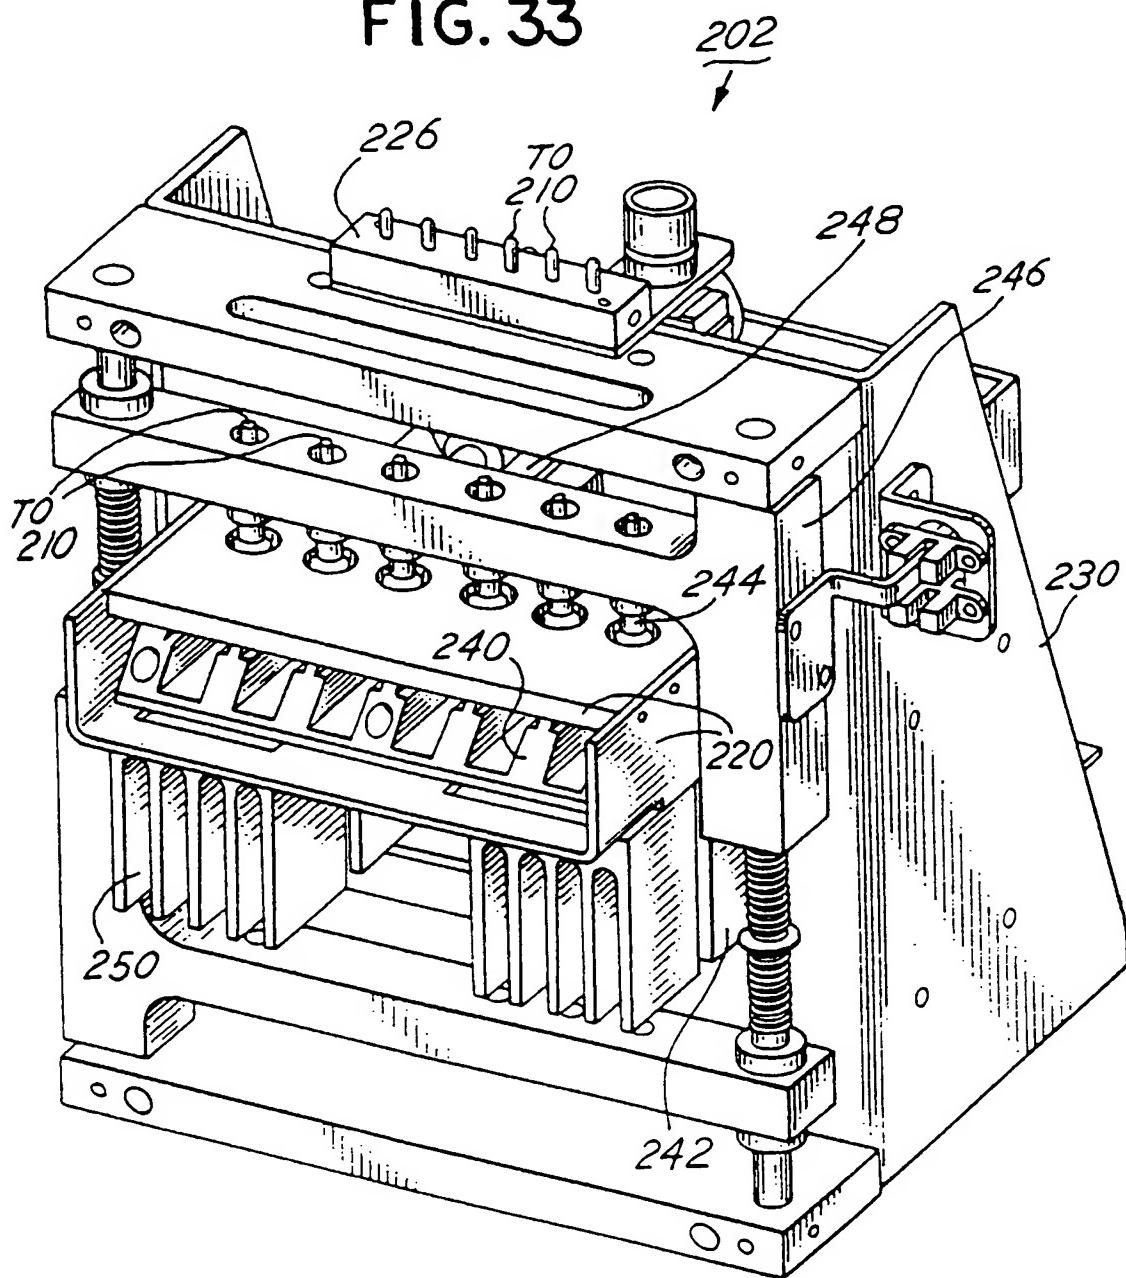


FIG.34

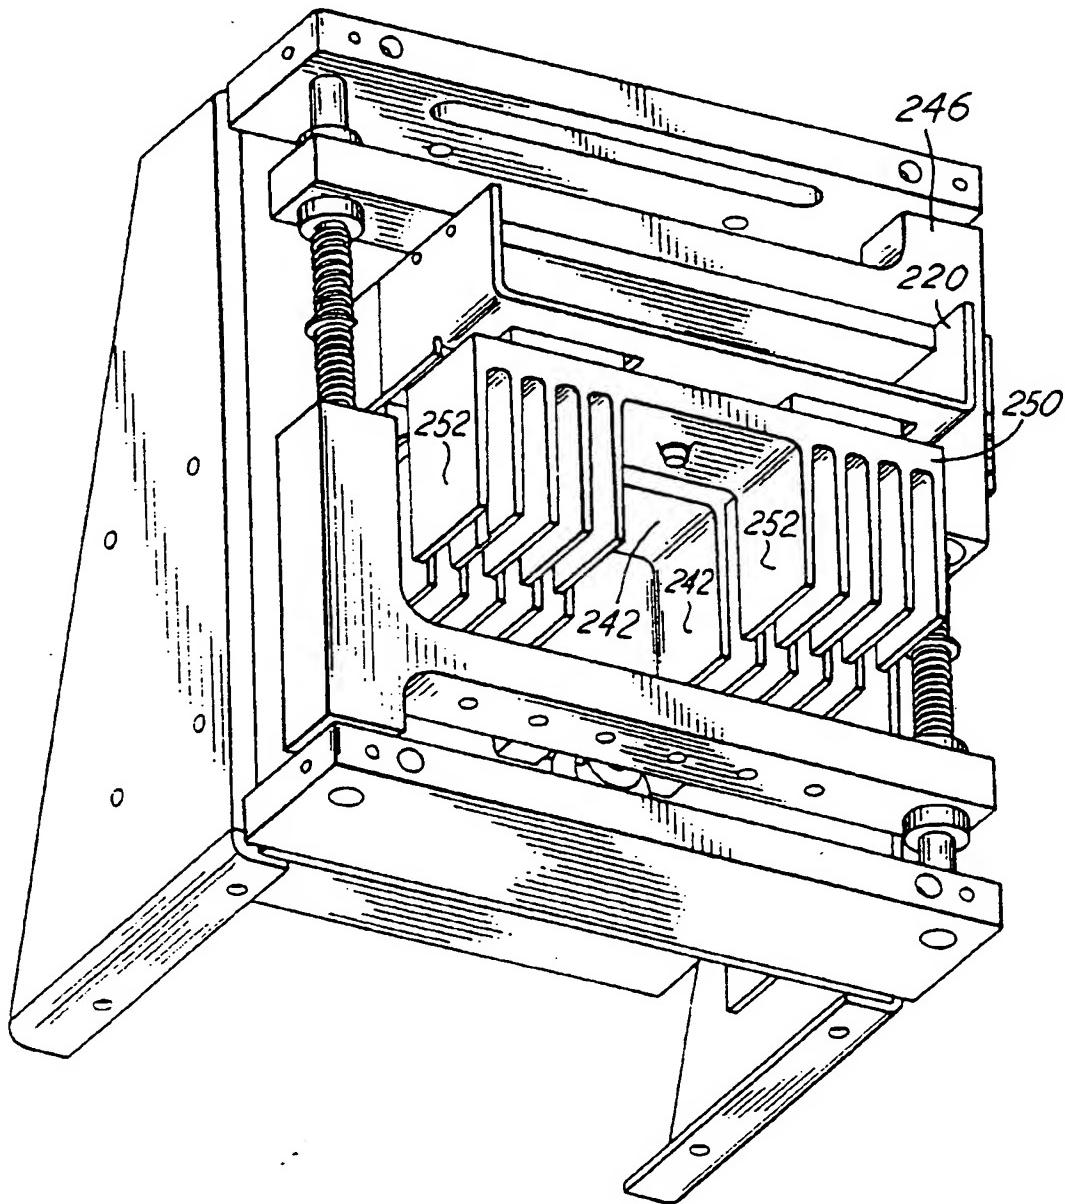


FIG.35

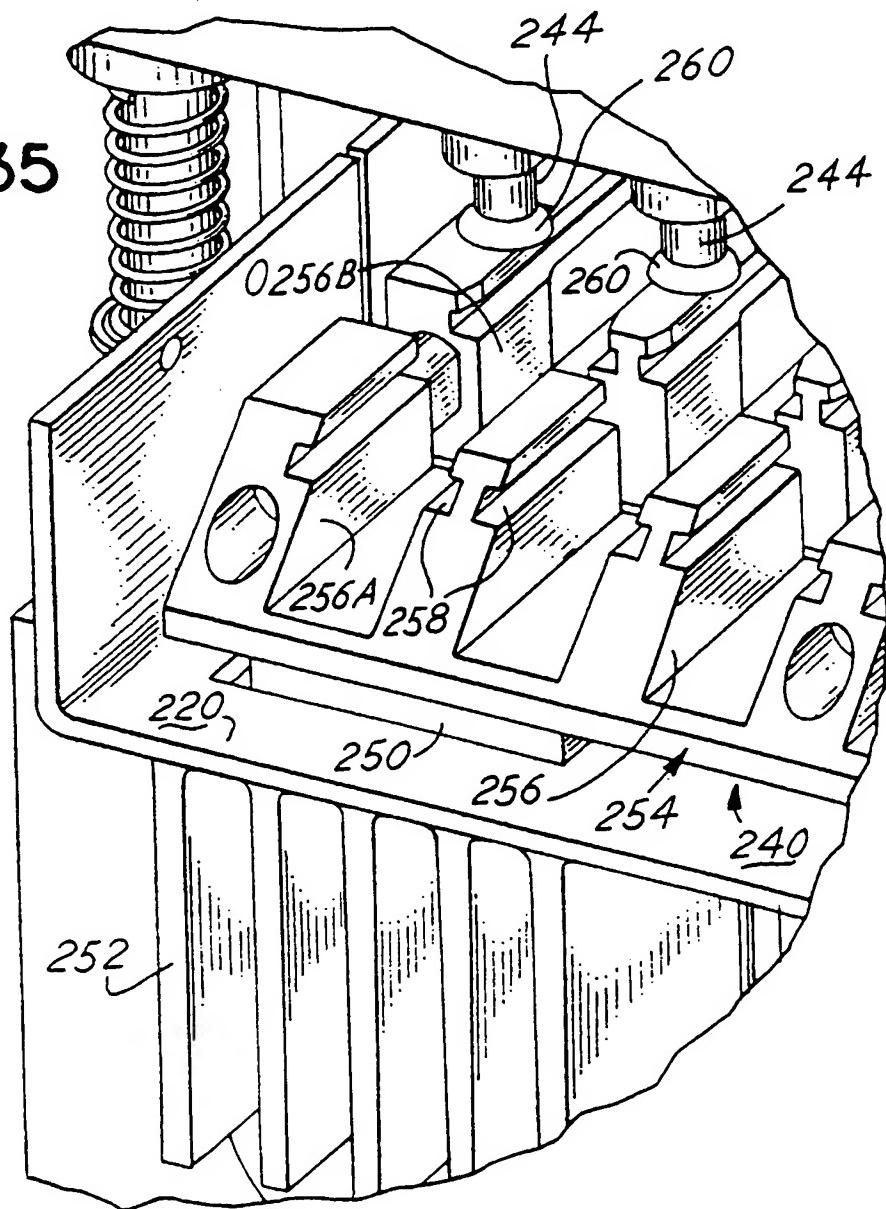


FIG. 36

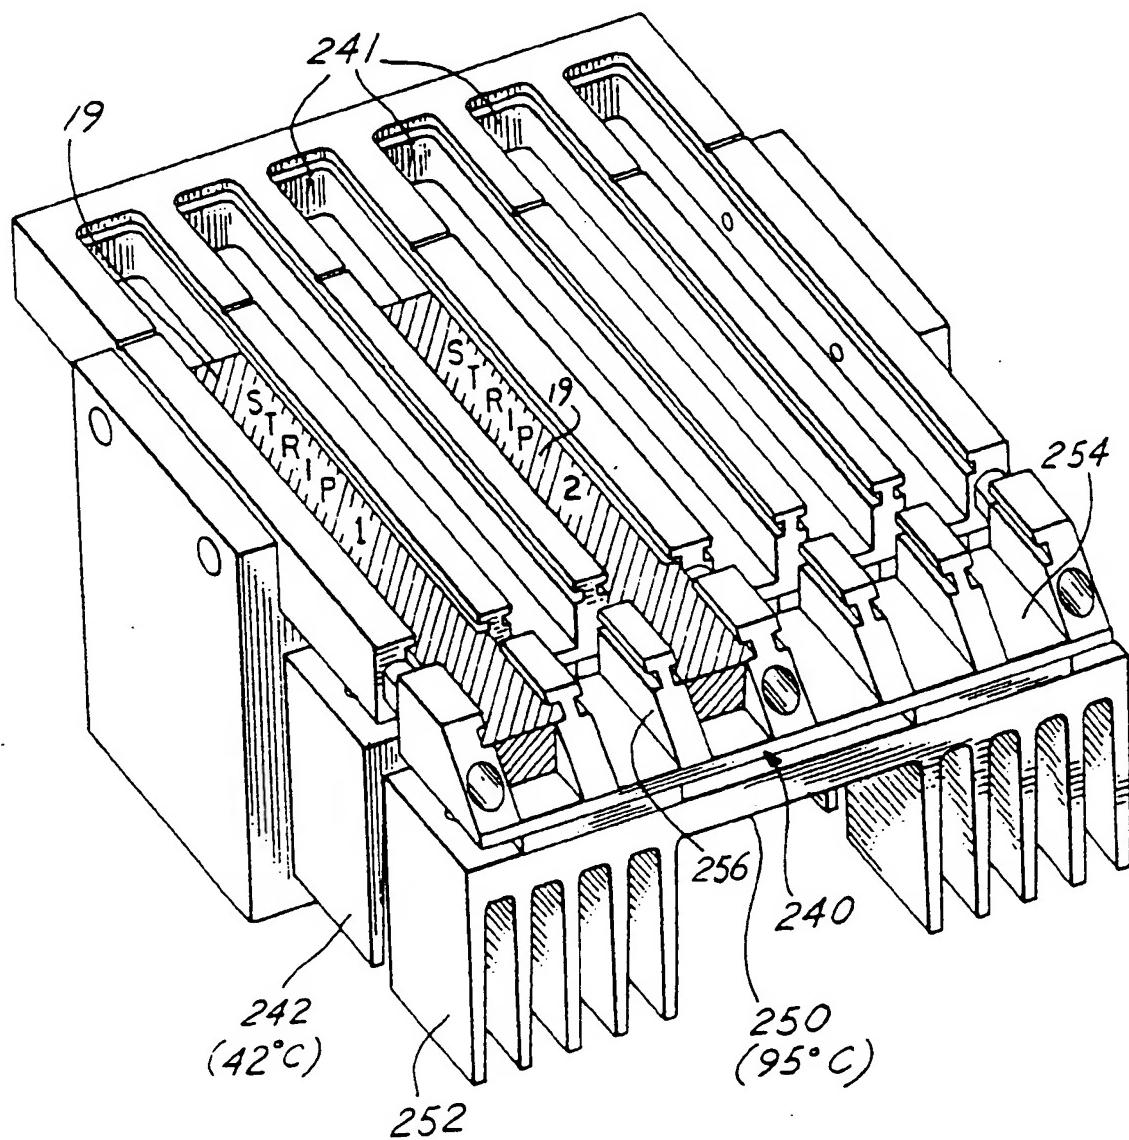


FIG. 37

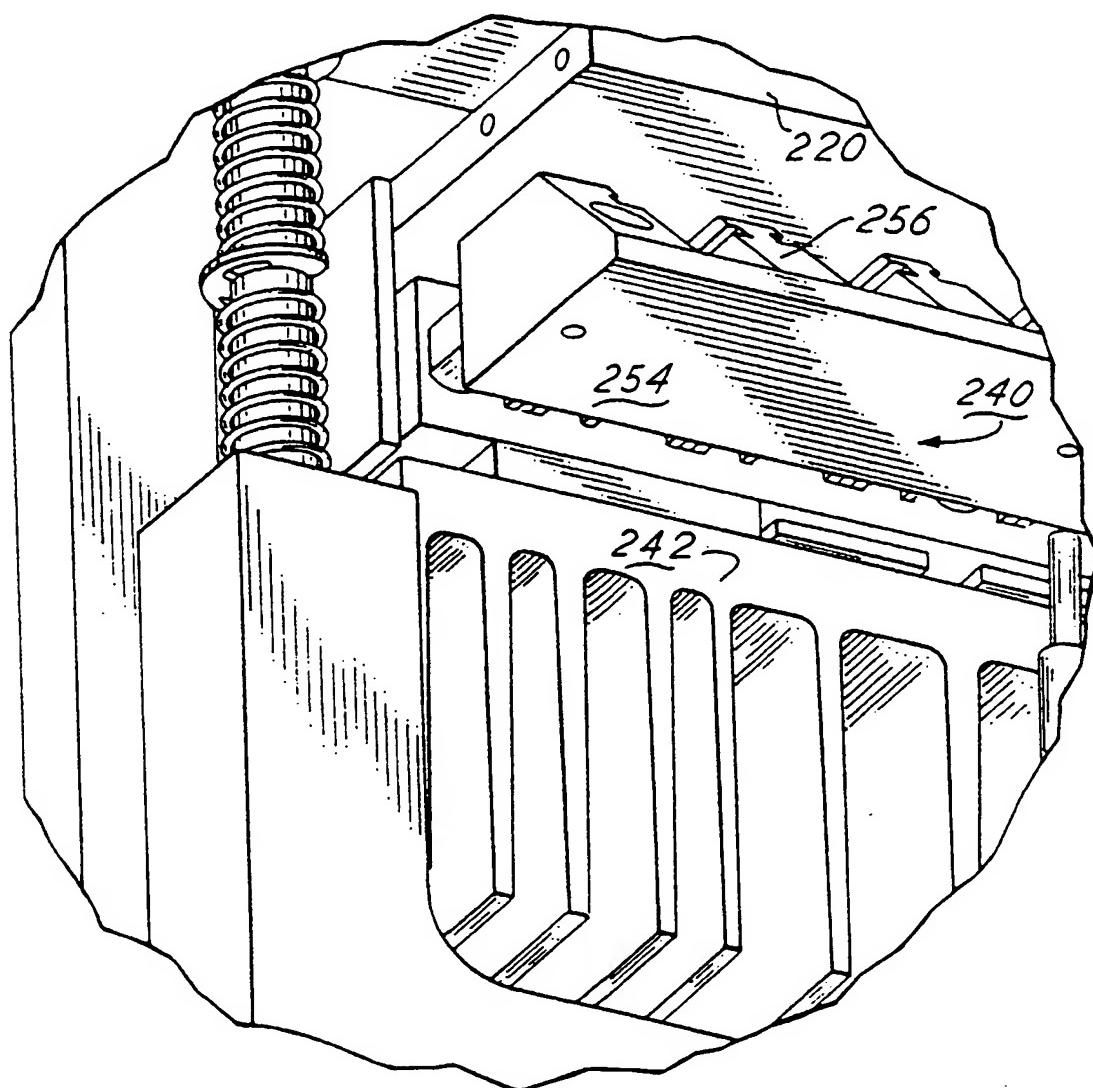


FIG. 38

AMPLIFICATION STATION (BLOCKS DIAGRAM)

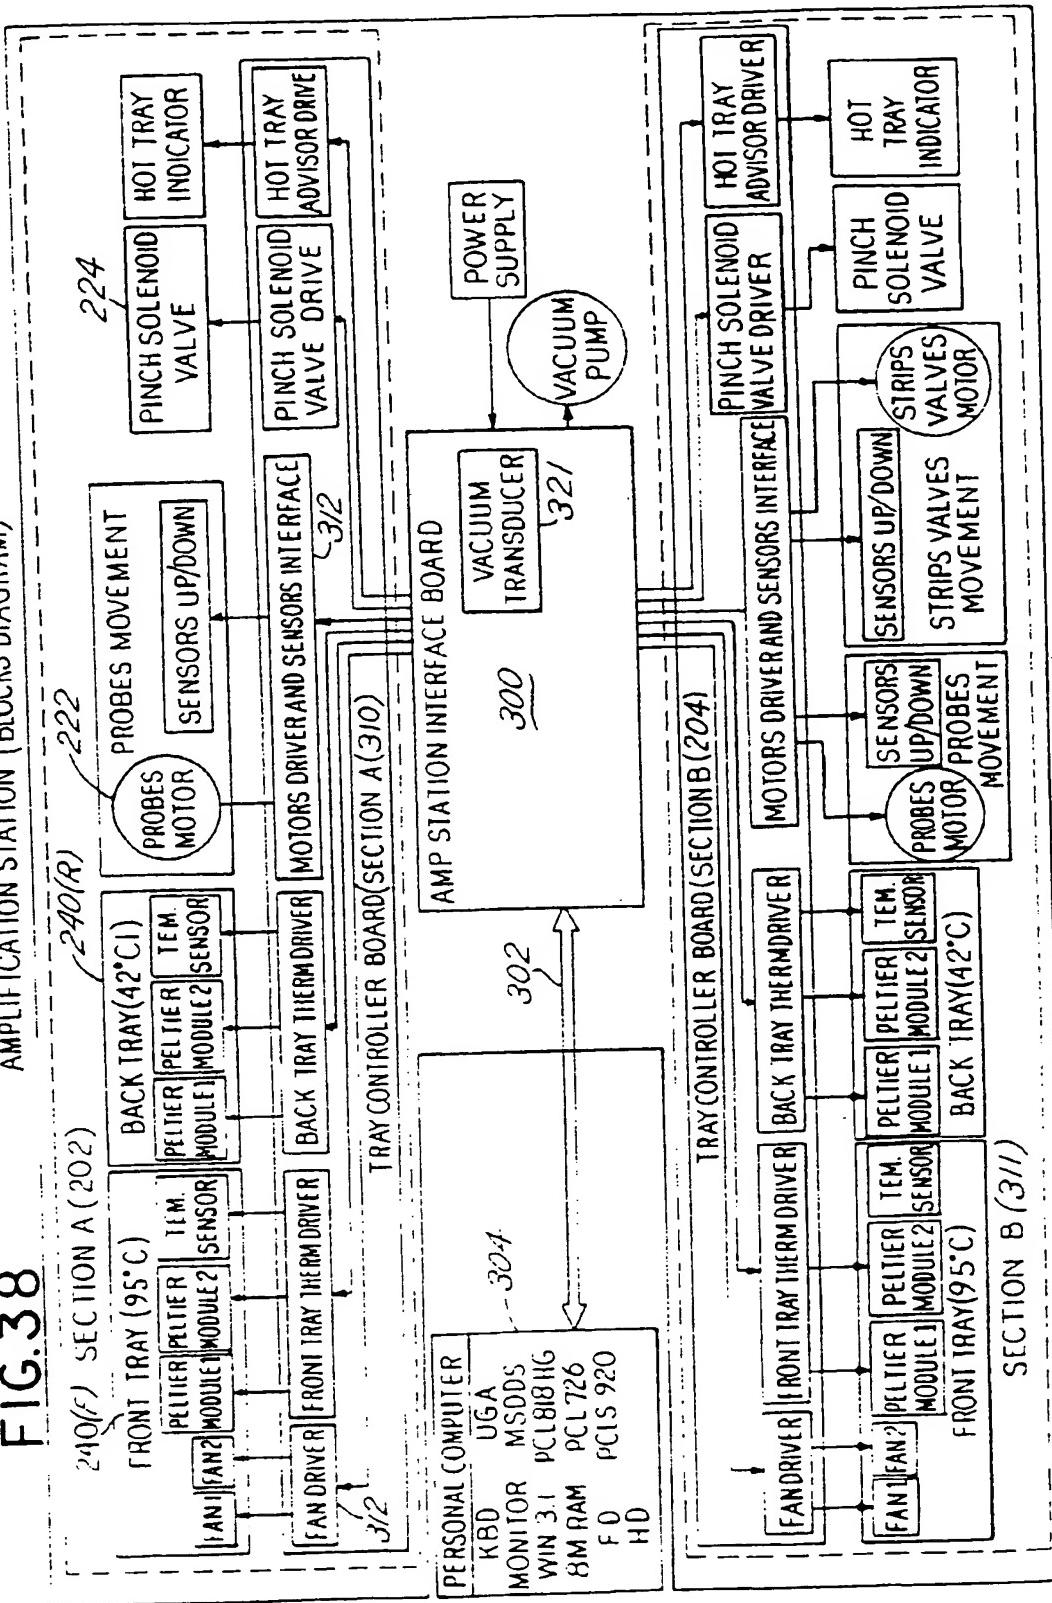


FIG. 39
VACUUM SYSTEM DIAGRAM

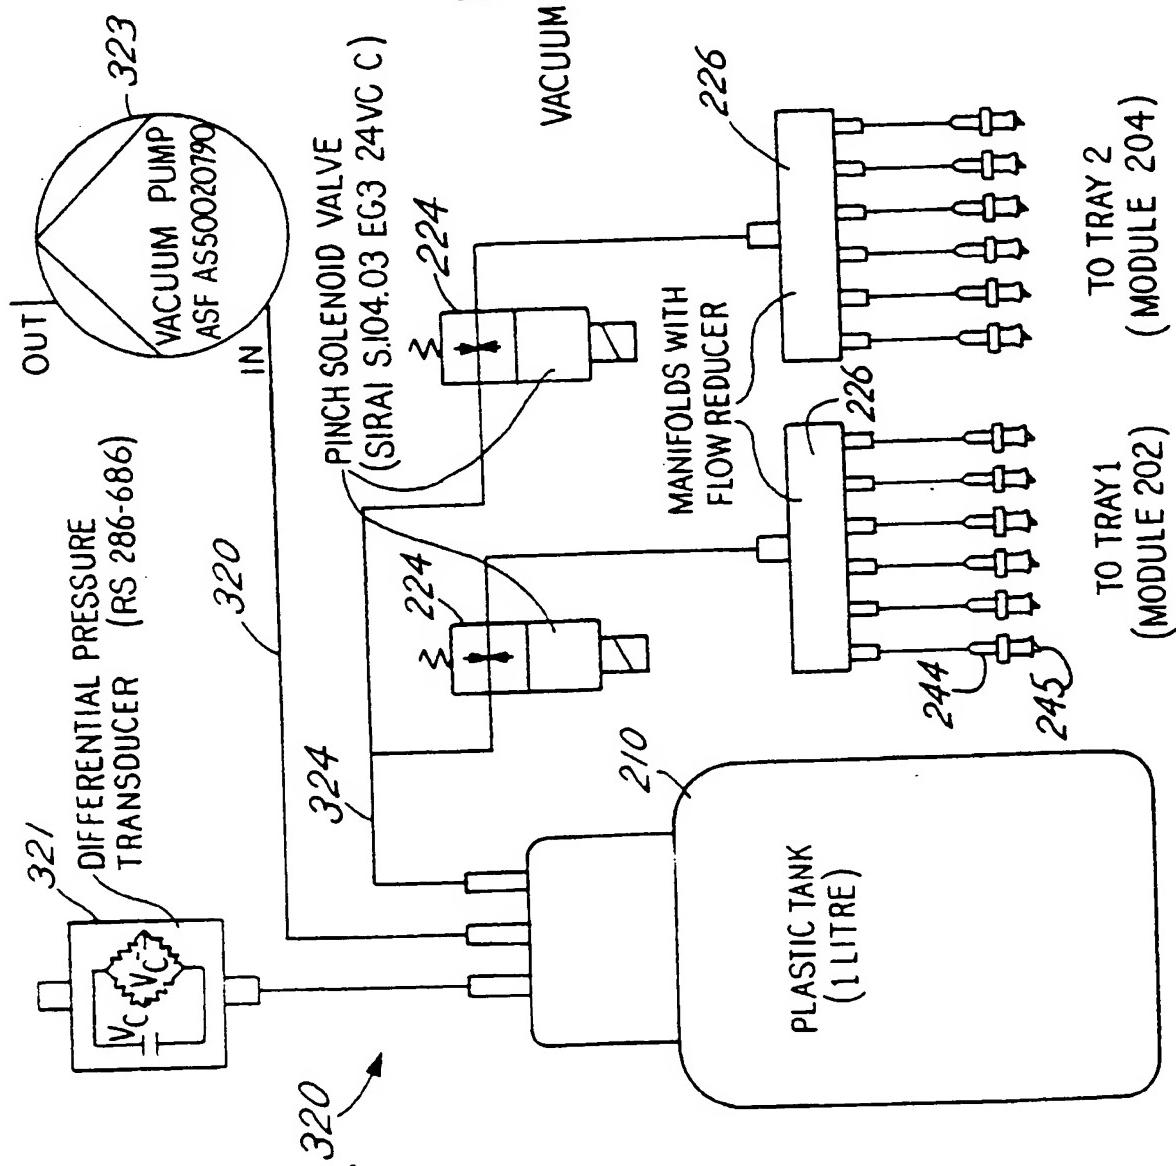


FIG.40

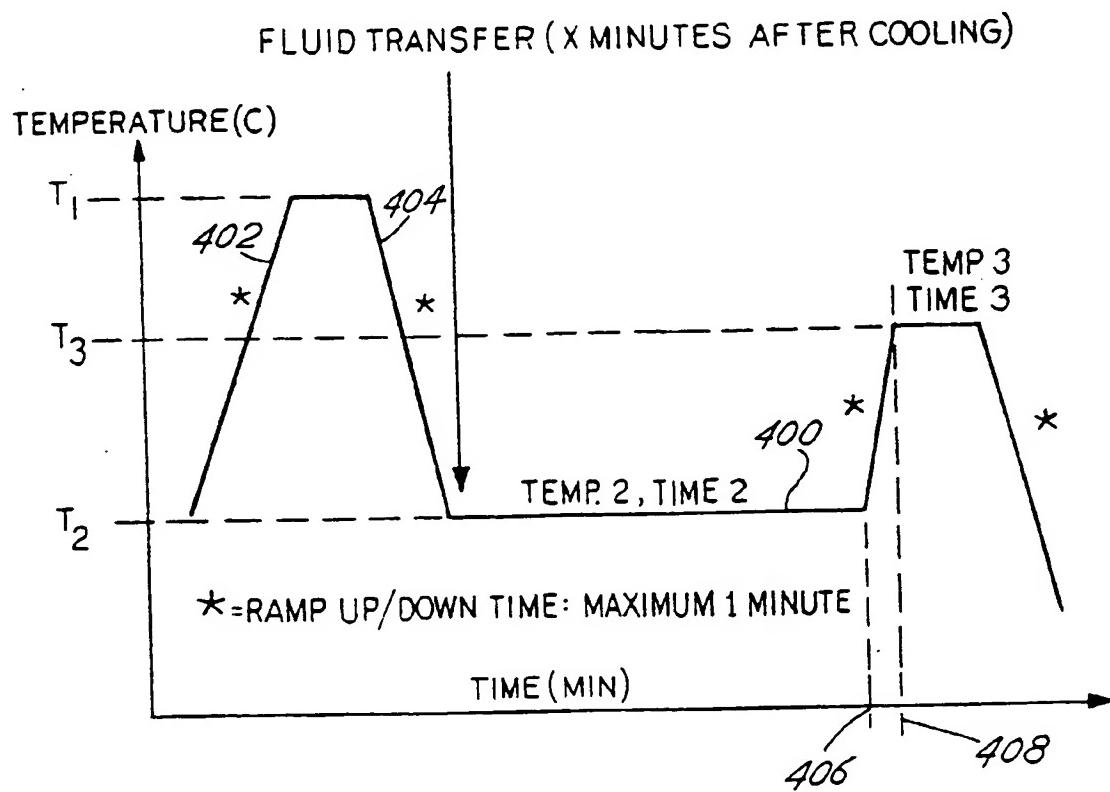


FIG.41

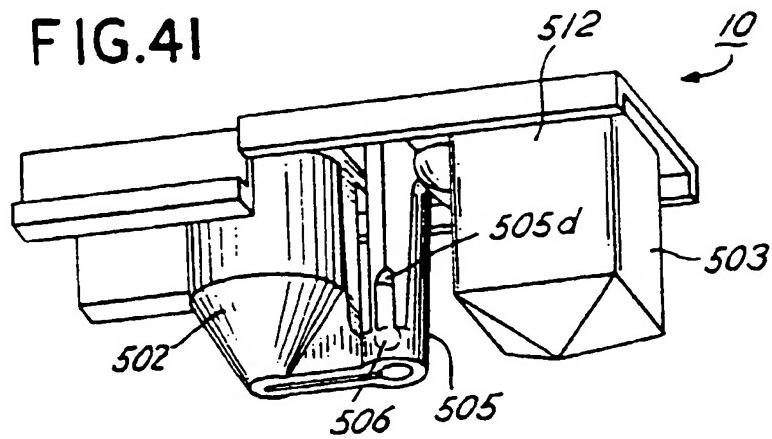


FIG.42

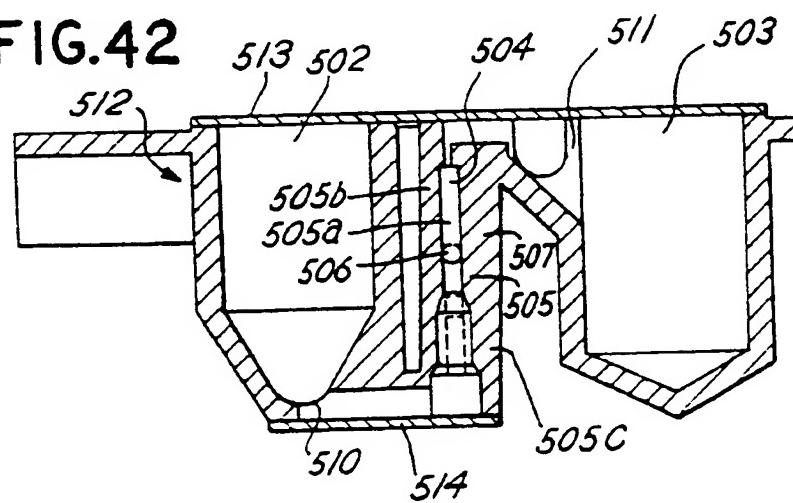


FIG.43

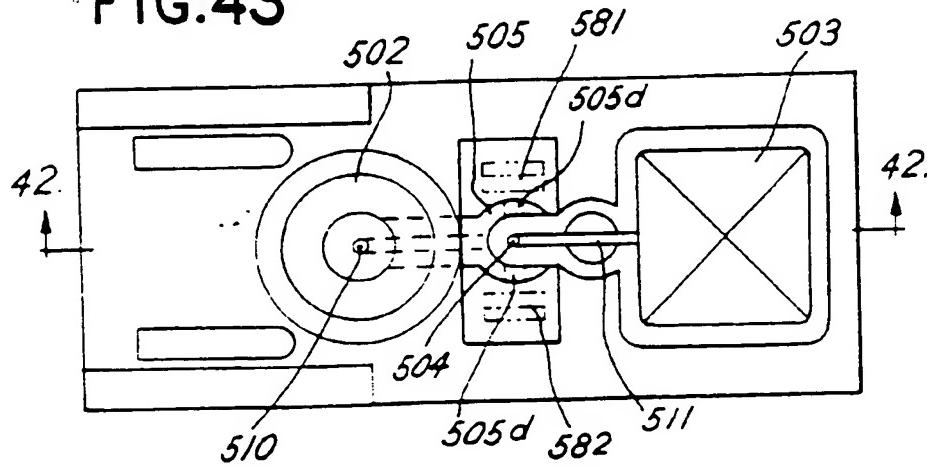


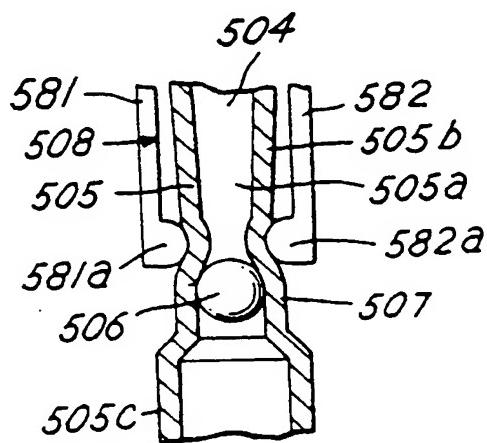
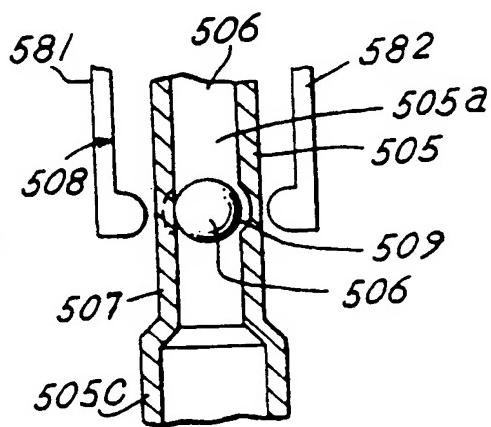
FIG.44**FIG.45**

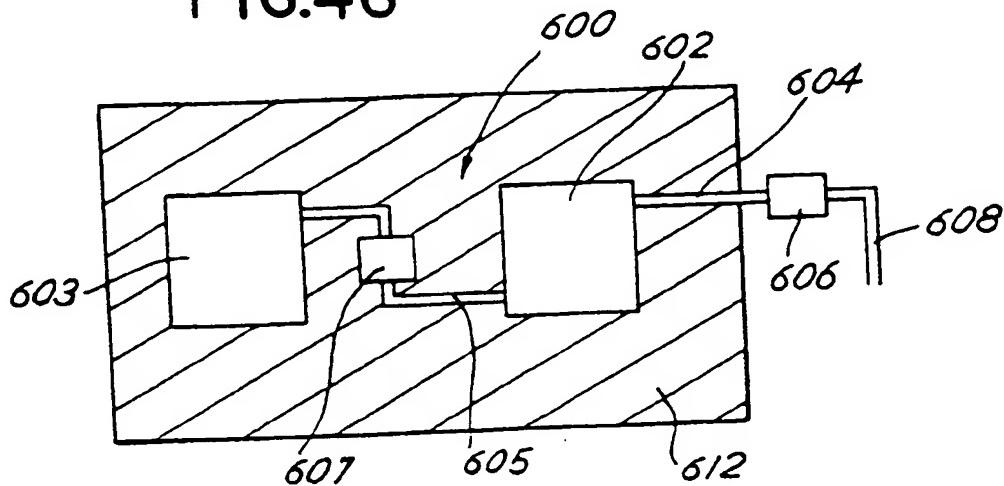
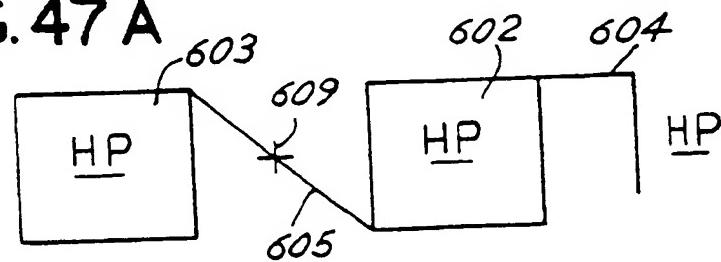
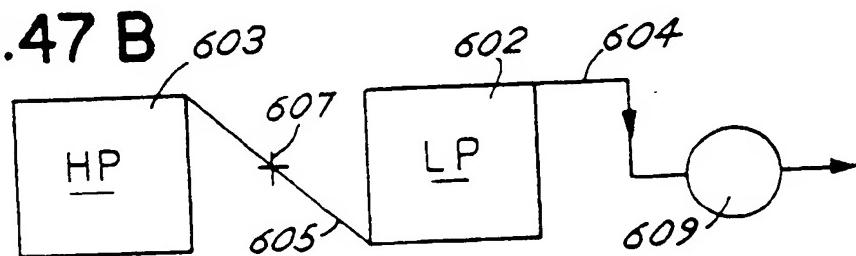
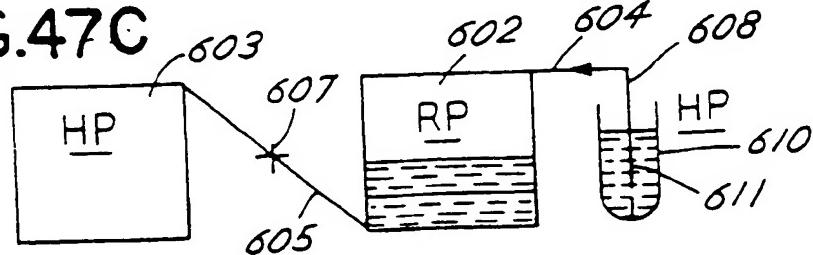
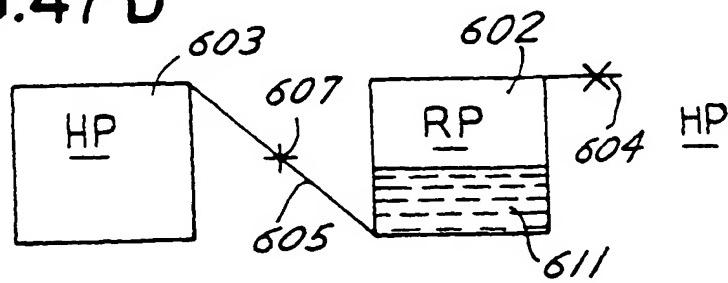
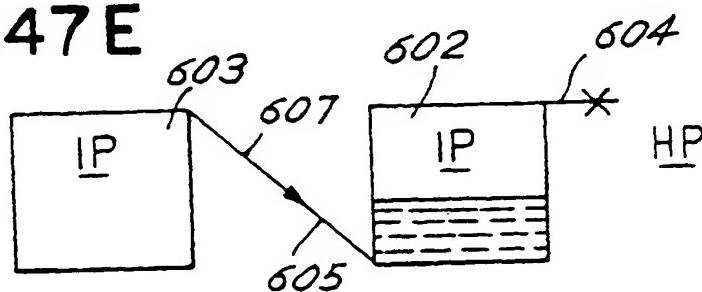
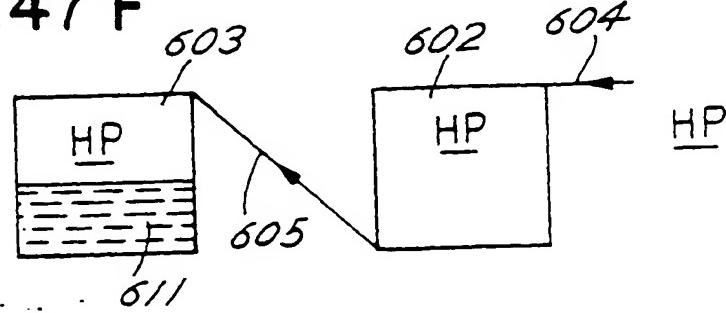
FIG.46**FIG.47 A****FIG.47 B****FIG.47C**

FIG.47 D**FIG.47 E****FIG.47 F**



(12)

EUROPEAN PATENT APPLICATION

(88) Date of publication A3:
24.05.2000 Bulletin 2000/21

(51) Int Cl⁷: B01L 3/00
// C12Q1/68

(43) Date of publication A2:
04.11.1998 Bulletin 1998/45

(21) Application number: 98303296.2

(22) Date of filing: 28.04.1998

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE
Designated Extension States:
AL LT LV MK RO SI

(30) Priority: 02.05.1997 US 850207
02.04.1998 US 53823

(71) Applicant: bioMerieux Vitek, Inc.
Hazelwood, Missouri 63042-2905 (US)

(72) Inventors:

- Catanzariti,Luigi
Duxbury, Massachusetts 02332 (US)
- Klutzz,Bryan W.
Norwell, Massachusetts (US)
- McKinley,Geoff A.
Duxbury, Massachusetts (US)
- Garland,Arthur L.
Carver, Massachusetts 02330 (US)

- Graziano,Louis
Rockland, Massachusetts 02370 (US)
- Moe,James G.
Franklin, Massachusetts 02038 (US)
- Vera-Garcia,Marcela
Framingham, Massachusetts 01702 (US)
- Bishop,James Clement
Columbia, Missouri 65203 (US)
- Chastain,David
Acton, Massachusetts 01720 (US)
- Gennari,Fabio
58 50015 Ponte A EMA, Florence (IT)
- Colin,Bruno
69280 Marcy L'Etoile (FR)
- Jaravel,Cecile
69003 Lyon (FR)

(74) Representative: Froud, Clive et al
Elkington and Fife
Prospect House
8 Pembroke Road
Sevenoaks, Kent TN13 1XR (GB)

(54) Dual chamber disposable reaction vessel for amplification reactions, reaction processing station therefor, and methods of use

(57) A reaction vessel for a nucleic acid amplification reaction has a first chamber containing an amplification reagent mix, a second chamber containing an amplification enzyme, and a fluid channel or chamber connecting the first and second chambers together. A fluid sample is introduced into the first chamber. After a denaturation and primer annealing process has occurred in the first chamber, the fluid chamber is opened to allow the solution of the reagent and fluid sample to flow into the second chamber. The second chamber is maintained at an optimal temperature for the amplification reaction.

A station is described for processing test strips incorporating the reaction vessels. The station includes temperature and vacuum control subsystems to maintain proper temperatures in the reaction vessel and effectuate the transfer of the fluid from one chamber to the other in an automated fashion without human interven-

tion.

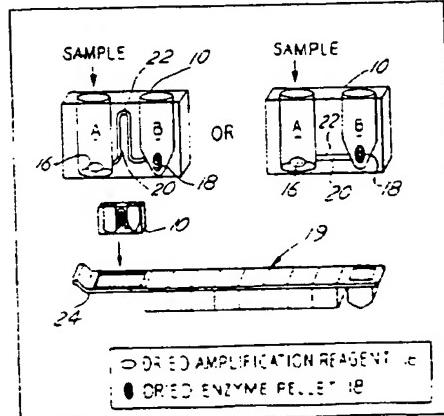


FIG.3



European Patent
Office

EUROPEAN SEARCH REPORT

Application Number

EP 98 30 3296

DOCUMENTS CONSIDERED TO BE RELEVANT			CLASSIFICATION OF THE APPLICATION (Int.Cl.)	
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	B01L3/00 //C12Q1/68	
Y	EP 0 674 009 A (BECTON DICKINSON CO) 27 September 1995 (1995-09-27) * column 5, line 8 - line 50; figures * * column 6, line 37 - column 7, line 24 * * column 10, line 35 - column 11, line 12 * * column 15, line 23 - line 56 * ---	1,2,4,21	B01L3/00 //C12Q1/68	
Y	US 5 554 516 A (KACIAN DANIEL L ET AL) 10 September 1996 (1996-09-10)	1,2,4,21		
A	* column 5, line 31 - line 44 *	22		
A	US 3 994 594 A (SANDROCK HAROLD E ET AL) 30 November 1976 (1976-11-30) * column 11, line 67 - column 12, line 26; figure 19 * * column 2, line 64 - column 3, line 16; figures *	3		
A	FR 2 612 297 A (PASTEUR DIAGNOSTICS) 16 September 1988 (1988-09-16)	3,11	TECHNICAL FIELDS SEARCHED (Int.Cl.)	
A	* page 7, line 34 - line 37 * * page 6, line 1 - page 7, line 8; figures 18-23 * * page 12, line 24 - line 28 *	21	B01L	
A	US 5 229 297 A (SCHNIPELSKY PAUL N ET AL) 20 July 1993 (1993-07-20)	1,3,12		
A	* column 9, line 26 - line 32 * * column 10, line 13 - line 19 * * column 10, line 47 - line 61; figure 1 * * column 14, line 61 - line 68; figures 9-13 * * column 16, line 3 - line 7 *	1		
	---	-/-		
The present search report has been drawn up for all claims				
Place of search	Date of completion of the search	Examiner		
THE HAGUE	21 March 2000	HOCQUET, A		
CATEGORY OF CITED DOCUMENTS				
X	particularly relevant if taken alone	T	theory or principle underlying the invention	
Y	particularly relevant if combined with another document of the same category	E	earlier patent document, but published on, or after the filing date	
A	technological background	D	document cited in the application	
O	non-written disclosure	L	document cited for other reasons	
P	intermediate document	S	member of the same patent family, corresponding document	

European Patent
Office

Application Number

EP 98 30 3296

CLAIMS INCURRING FEES

The present European patent application comprised at the time of filing more than ten claims.

- Only part of the claims have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims and for those claims for which claims fees have been paid, namely claim(s):
- No claims fees have been paid within the prescribed time limit. The present European search report has been drawn up for the first ten claims.

LACK OF UNITY OF INVENTION

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

see sheet B

- All further search fees have been paid within the fixed time limit. The present European search report has been drawn up for all claims.
- As all searchable claims could be searched without effort justifying an additional fee, the Search Division did not invite payment of any additional fee.
- Only part of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the inventions in respect of which search fees have been paid, namely claims:
- None of the further search fees have been paid within the fixed time limit. The present European search report has been drawn up for those parts of the European patent application which relate to the invention first mentioned in the claims, namely claims:



European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 98 30 3296

DOCUMENTS CONSIDERED TO BE RELEVANT		Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.6)
Category	Citation of document with indication, where appropriate, of relevant passages		
A	EP 0 726 310 A (GEN PROBE INC) 14 August 1996 (1996-08-14) * page 3, line 24 - line 39 * * page 5, line 29 - line 55 * ---	1-12,21, 22	
A	WO 97 03348 A (IMMUNOLOGICAL ASSOCIATES OF DE) 30 January 1997 (1997-01-30) * page 15, line 10 - page 16, line 23; figure 1 *	1,3	
A	WO 95 34684 A (UNIV GEORGETOWN) 21 December 1995 (1995-12-21) * page 6, line 18 - line 25 * * page 29, line 18 - page 30, line 2 * ---	1-11,21	
A	EP 0 573 098 A (EASTMAN KODAK CO) 8 December 1993 (1993-12-08) * figures *	11	
A	US 3 579 303 A (PICKERING DONALD E) 18 May 1971 (1971-05-18) * column 5, line 69 - column 6, line 20; figure 11 *	5	TECHNICAL FIELDS SEARCHED (Int.Cl.6)
A	US 4 332 769 A (RAMPY GORDON A ET AL) 1 June 1982 (1982-06-01) * column 2, line 5 - line 41 * * column 2, line 53 - column 3, line 35 * ---	5	
A	EP 0 693 560 A (BECTON DICKINSON CO) 24 January 1996 (1996-01-24) * column 11, line 19 - line 48; figure 7A * * column 13, line 41 - line 57; figure 10 * * column 16, line 49 - column 17, line 36; figure 15 *	13	
		-/-	
<p>The present search report has been drawn up for all claims</p>			
Place of search	Date of completion of the search	Examiner	
THE HAGUE	21 March 2000	HOCQUET, A	
CATEGORY OF CITED DOCUMENTS		T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons & : member of the same patent family, corresponding document	
X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document			

EP 0 875 291 A3 1.1

European Patent
OfficeLACK OF UNITY OF INVENTION
SHEET BApplication Number
EP 98 30 3296

The Search Division considers that the present European patent application does not comply with the requirements of unity of invention and relates to several inventions or groups of inventions, namely:

1. Claims: 1-4,11,12,19,21,22

dual chamber reaction vessel with means for fluid communication between the chambers, amplification reagents in the first chamber and enzymes in the second chamber, strip comprising the vessel, method for conducting nucleic acid amplification using the vessel.

2. Claims: 5-10,18

dual chamber reaction vessel with a flexible conduit linking the two chambers, a rigid seal piece in the conduit, and an external constricting device creating a passage in said conduit.

3. Claims: 13-17

nucleic acid amplification station

4. Claim : 20

test strip with an aperture for receiving an amplification vessel

5. Claim : 23

process for transferring a liquid between chambers by controlling the relative pressure of the chambers.



European Patent
Office

EUROPEAN SEARCH REPORT

Application Number

EP 98 30 3296

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.CI.6)
A	EP 0 636 413 A (PERKIN ELMER CORP) 1 February 1995 (1995-02-01) * column 21, line 15 - line 26 * * column 22, line 18 - line 25; figure 12 * * column 23, line 44 - line 53; figures 16-19 * * column 24, line 53 - column 25, line 20; figure 20 * ---	13	
X	WO 95 11083 A (ABBOTT LAB) 27 April 1995 (1995-04-27) * page 15, line 5 - line 18 * * page 17, line 17 - page 18, line 9; figure 7 *	20	
A	US 5 605 665 A (CLARK FREDERIC L ET AL) 25 February 1997 (1997-02-25) * column 52, line 26 - column 53, line 28; figure 45 *	20	
A	WO 97 02357 A (AFFYMETRIX INC ;ANDERSON ROLFE C (US); LIPSHUTZ ROBERT J (US); RAV) 23 January 1997 (1997-01-23) * page 46, line 23 - page 50, line 29; figure 6 *	23	TECHNICAL FIELDS SEARCHED (Int.CI.6)
The present search report has been drawn up for all claims			
Place of search THE HAGUE	Date of completion of the search 21 March 2000	Examiner HOCQUET, A	
CATEGORY OF CITED DOCUMENTS		T theory or principle underlying the invention E earlier patent document, but published on, or after the filing date D document cited in the application L document cited for other reasons & . member of the same patent family, corresponding document	
X particularly relevant if taken alone Y particularly relevant if combined with another document of the same category A technological background O non-written disclosure P intermediate document			

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 98 30 3296

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
 The members are as contained in the European Patent Office EOP file on
 The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-03-2000

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
EP 0674009	A	27-09-1995	AU 689187 B AU 1352595 A BR 9501042 A CA 2143365 A JP 2675989 B JP 7265100 A SG 30306 A US 5725831 A US 5783148 A	26-03-1998 21-09-1995 31-10-1995 15-09-1995 12-11-1997 17-10-1995 01-06-1996 10-03-1998 21-07-1998
US 5554516	A	10-09-1996	US 5888729 A AU 681082 B AU 4222493 A AU 711448 B AU 4523897 A CA 2135073 A EP 0587266 A JP 7506255 T WO 9322461 A	30-03-1999 21-08-1997 29-11-1993 14-10-1999 19-02-1998 11-11-1993 16-03-1994 13-07-1995 11-11-1993
US 3994594	A	30-11-1976	AU 500840 B AU 1723176 A AU 5041379 A BE 844663 A CA 1079540 A CA 1070139 A CH 611028 A DE 2636678 A FR 2322368 A GB 1538143 A IT 1069664 B JP 52029271 A NL 7608413 A SE 7609323 A SU 640682 A US 4083638 A	31-05-1979 02-03-1978 03-01-1980 31-01-1977 17-06-1980 22-01-1980 15-05-1979 10-03-1977 25-03-1977 10-01-1979 25-03-1985 04-03-1977 01-03-1977 28-02-1977 30-12-1978 11-04-1978
FR 2612297	A	16-09-1988	NONE	
US 5229297	A	20-07-1993	CA 1338505 A DE 69009510 D DE 69009510 T DK 381501 T EP 0381501 A FI 94360 B IE 63501 B	06-08-1996 14-07-1994 05-01-1995 04-07-1994 08-08-1990 15-05-1995 03-05-1995

EPO - NM DMS
 For more details about this annex see Official Journal of the European Patent Office, No 2/82

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 98 30 3296

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
 The members are as contained in the European Patent Office EDP file on
 The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-03-2000

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5229297 A		JP 2536945 B JP 3007571 A KR 161276 B AT 130373 T AU 1664092 A DE 69206080 D DE 69206080 T EP 0530357 A ES 2081613 T FI 925285 A JP 8030704 B WO 9216659 A	25-09-1996 14-01-1991 16-11-1998 15-12-1995 21-10-1992 21-12-1995 13-06-1996 10-03-1993 01-03-1996 20-11-1992 27-03-1996 01-10-1992
EP 0726310 A	14-08-1996	US 5556771 A AU 699590 B AU 4916796 A CA 2210584 A JP 10503383 T WO 9624664 A US 5614387 A US 5834254 A	17-09-1996 10-12-1998 27-08-1996 15-08-1996 31-03-1998 15-08-1996 25-03-1997 10-11-1998
WO 9703348 A	30-01-1997	AU 6458096 A CA 2226717 A EP 0838025 A JP 11509100 T US 5955351 A	10-02-1997 30-01-1997 29-04-1998 17-08-1999 21-09-1999
WO 9534684 A	21-12-1995	AU 692792 B AU 7512394 A JP 10505224 T	18-06-1998 05-01-1996 26-05-1998
EP 0573098 A	08-12-1993	US 5364591 A CA 2095591 A,C DE 69309152 D DE 69309152 T FI 932502 A JP 6046828 A	15-11-1994 02-12-1993 30-04-1997 18-09-1997 02-12-1993 22-02-1994
US 3579303 A	18-05-1971	CA 937910 A US 3561186 A	04-12-1973 09-02-1971
US 4332769 A	01-06-1982	NONE	
EP 0693560 A	24-01-1996	US 5639428 A AU 2331095 A	17-06-1997 01-02-1996

For more details about this annex see Official Journal of the European Patent Office, No 12/82

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 98 30 3296

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-03-2000

Patent document cited in search report	Publication date		Patent family member(s)	Publication date
EP 0693560 A			BR 9503364 A CA 2152307 A JP 8062225 A SG 32408 A	27-02-1996 20-01-1996 08-03-1996 13-08-1996
EP 0636413 A	01-02-1995		JP 7075544 A US 6033880 A US 5720923 A US 5827480 A US 5779977 A	20-03-1995 07-03-2000 24-02-1998 27-10-1998 14-07-1998
WO 9511083 A	27-04-1995		AU 8123594 A CA 2173861 A EP 0724483 A JP 9504690 T US 5753186 A US 5604101 A	08-05-1995 27-04-1995 07-08-1996 13-05-1997 19-05-1998 18-02-1997
US 5605665 A	25-02-1997		US 5376313 A AU 7843194 A CA 2172363 A EP 0720747 A JP 9503060 T WO 9508774 A US 5646049 A US 5635364 A US 5575978 A US 5627522 A US 5536471 A US 5507410 A US 5610069 A US 5960160 A US 5578494 A US 5762878 A AU 3929093 A AU 3934393 A AU 3934993 A AU 3935093 A AU 3967793 A AU 3968093 A CA 2129245 A CA 2129246 A CA 2129367 A CA 2129368 A CA 2132959 A CA 2132960 A	27-12-1994 10-04-1995 31-03-1995 10-07-1996 25-03-1997 30-03-1995 08-07-1997 03-06-1997 19-11-1996 06-05-1997 16-07-1996 16-04-1996 11-03-1997 28-09-1999 26-11-1996 09-06-1998 08-11-1993 08-11-1993 08-11-1993 08-11-1993 14-10-1993 14-10-1993 14-10-1993 14-10-1993 14-10-1993 14-10-1993

For more details about this annex see Official Journal of the European Patent Office, No 12/92

DOLY-FIRM-F49

ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.

EP 98 30 3296

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report. The members are as contained in the European Patent Office EDP file on. The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

21-03-2000

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 5605665 A		EP 0755519 A EP 0634016 A EP 0637283 A EP 0746769 A EP 0632894 A EP 0632896 A JP 7505473 T JP 7505474 T JP 2769245 B JP 7505475 T JP 7505343 T JP 7505476 T JP 7506184 T WO 9320440 A WO 9320444 A WO 9320443 A WO 9319928 A WO 9320441 A WO 9320450 A US 5358691 A US 5540890 A US 5482861 A	29-01-1997 18-01-1995 08-02-1995 11-12-1996 11-01-1995 11-01-1995 15-06-1995 15-06-1995 25-06-1998 15-06-1995 15-06-1995 15-06-1995 06-07-1995 14-10-1993 14-10-1993 14-10-1993 14-10-1993 14-10-1993 25-10-1994 30-07-1996 09-01-1996
WO 9702357 A	23-01-1997	US 5856174 A AU 6404996 A EP 0843734 A JP 11509094 T US 5922591 A	05-01-1999 05-02-1997 27-05-1998 17-08-1999 13-07-1999

EPC/CPA/03159

For more details about this annex see Official Journal of the European Patent Office, No. 12/82